

# THERE FOR YOU.



**Products with outstanding quality**  
cutting edge technology manufactured by us



**Consistent reliability and support**  
dependable service beyond product sales



**Constant Innovation**  
creating solutions for emerging needs

That is the

**RITA LEIBINGER GUARANTEE.**



LeiLOX TPLO



TTA RAPID®



Tiny

for smaller patients

LeiLOX TPLO SWING



RAPID LUXATION




LeiLOX CBLO

**CRUCIATE LIGAMENT REPAIR & PATELLA LUXATION SYSTEMS**

*Knee and Patella*

LeiLOX CCWO

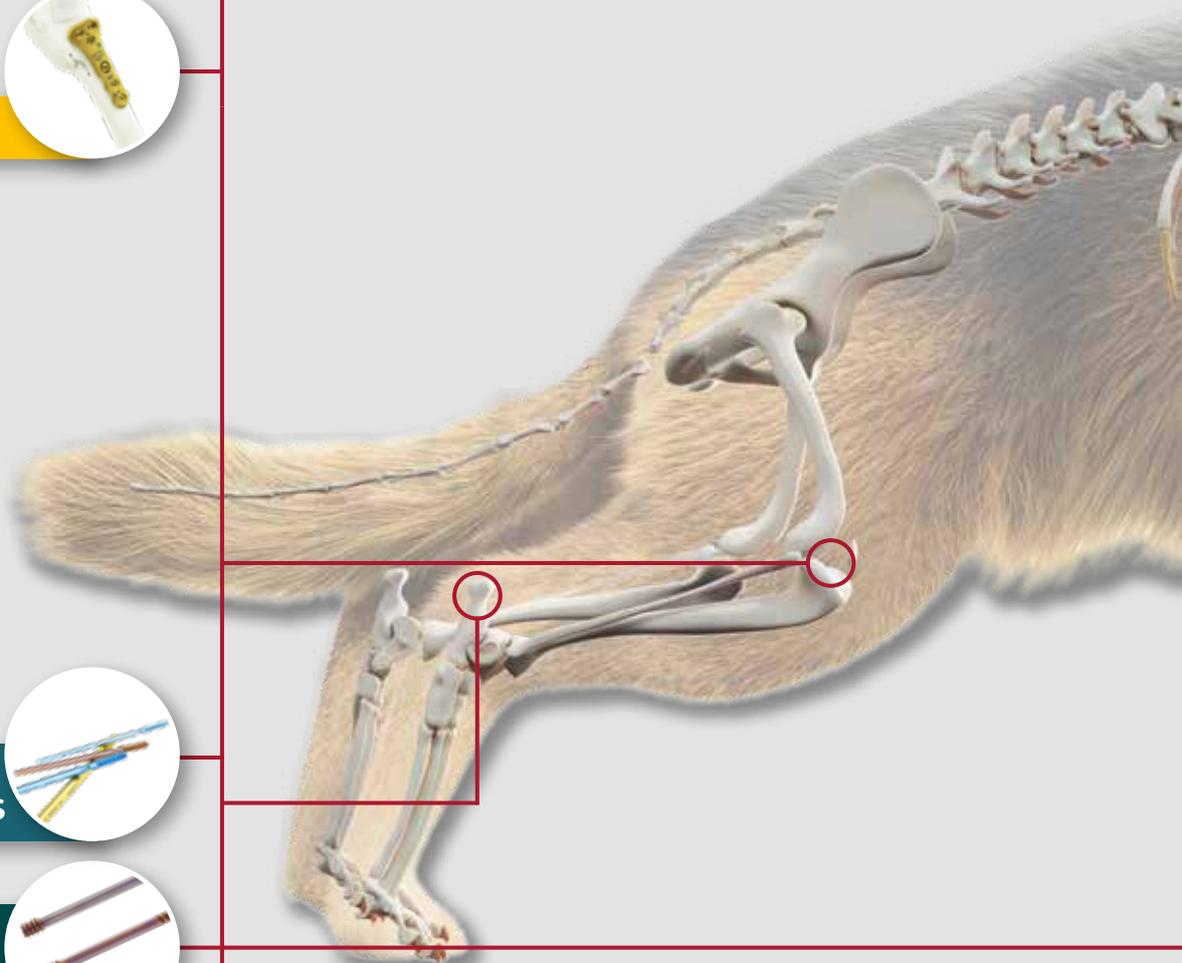

**FIXATION & COMPRESSION SYSTEMS**

*General Application*

SUTURES & BONE ANCHORS

LeiCOM COMPRESSION SCREWS



**BONE SUBSTITUTE**  
*General Application*

LeiLa **BONE MATTER**

# OUR PRODUCTS



**LeiMESH**  
Dynamic Cuttable Mesh System

Cranial Trauma, Bone Cement Augmentation, Reconstruction, Oral Surgery, etc.



**LeiLOX 1.0/1.3**  
Nano Locking System



**LeiLOX 1.5/2.0**  
Micro Locking System



**LeiLOX 2.0-3.5**  
Locking System

## FRACTURE TREATMENT

Humerus, Radius, Femur, Tibia, etc.



## CERVICAL REPAIR

**C-LOX SPINAL**  
Intervertebral Fusion Distraction



## ARTHROSCOPIC INSTRUMENTS

**SMALL ANIMAL ARTHRO.**  
Van Ryssen Series



**EQUINE DENTAL PLUGS**



**EQUINE ARTHROSCOPY**



# Learn from the Experts

Experience and knowledge are essential for successful surgeries. We provide you with our all-out support.

Learn from the best and hone your skills in one of our Continuing Education (CE) Courses / Workshops, Online Courses and Webinars, or a personal one-on-one.

Our CE Courses and Workshops are held by renowned experts and clinicians at locations all over the world, and cover everything from the fundamentals to advanced procedures.

Take a look at the range of educational courses we offer at the RITA LEIBINGER Academy website page.

## Visit our Academy Page

[leibinger.vet/academy](http://leibinger.vet/academy)

## Register for our Courses

[leibinger.vet/academy/#registration](http://leibinger.vet/academy/#registration)

## Contact Us

[info@leibinger-medical.com](mailto:info@leibinger-medical.com)



# NEW

FROM RITA LEIBINGER



## LeiLOX CCWO

With our new Titanium LeiLOX CCWO, we offer yet another reliable system in treating Cruciate Ligament Ruptures. This straightforward technique is specially suitable for juvenile patients and patients with very steep TPAs

## LeiLOX 1.0/1.3

Our Titanium LeiLOX Fracture Locking Plate System is specially developed for the smallest patients, such as Toy Breeds, Rodents, and Birds.



## LeiMESH

This highly versatile 3d Dynamic Cuttable Mesh System made of Titanium can be used for cranial or maxillofacial fractures after trauma, or reconstruction after tumors, as well as mandibular cases.

<b>Joint</b>	<b>TTA RAPID®</b>	TTA RAPID® Giant TTA RAPID® Standard TTA RAPID® Tiny <i>System Instruments</i>	TTA RAPID®
	<b>PATELLA LUXATION</b>	RAPID Luxation System <i>System Instruments</i>	Patella Luxation
	<b>TTA STANDARD</b>	Standard TTA Implants <i>Instruments</i>	TTA Standard
	<b>TPLO</b>	TPLO Locking, <i>Stainless Steel</i> TPLO Swing, <i>Titanium</i> TPLO Patella Luxation Spacers	TPLO
	<b>CBLO</b>	CBLO Locking, <i>Titanium</i>	CBLO
	<b>CCWO</b>	CCWO Locking, <i>Titanium</i>	CCWO
	<i>TPLO, CBLO, CCWO Instruments</i>		
<b>Osteosynthesis</b>	<b>LeiLOX 1.0/1.3</b>	1.0 /1.3 Nano Locking, <i>Titanium</i>	LeiLOX 1.0 / 1.3
	<b>LeiLOX 1.5/2.0</b>	1.5 /2.0 Micro Locking, <i>Titanium</i>	LeiLOX 1.5 / 2.0
	<b>LeiLOX 2.0-3.5</b>	LeiLOX, Locking 2.0/2.4, <i>Stainless Steel</i> LeiLOX, Locking 2.7/3.5, <i>Stainless Steel</i>	LeiLOX 2.0 -3.5
	<i>LeiLOX Instruments</i>		
	<b>General Osteosynthesis</b>	Standard Plates Screws (all) K-Wires, Orthopedic Cerclage	General Osteosynth.
	<b>LeiMESH</b>	Dynamic Cuttable Mesh System	Mesh System
	<b>LeiCOM</b>	Cannulated Compression Screws	LeiCOM Compression
	<b>LeiSU Sutures</b>	Suture Anchors, <i>Titanium</i> Sutures	Suture
<b>Spinal</b>	<b>C-LOX</b>	Cervical Intervertebral Fusion Implants, <i>Locking, Titanium</i>	C-LOX Spinal
<b>Bone Substitute</b>	<b>LeiLA</b>	Bone Graft Granules Hydroxyapatite Paste	Bone Matter
<b>Arthroscopy</b>	<b>Small Animal Arthroscopy</b> <b>Equine Arthroscopy</b>	Van Ryssen Series, Standard Wilderjans Design, Standard	Arthroscopy
<b>Dental</b>	<b>Equine Dental</b>	Dental Plugs, <i>Titanium</i>	Equine Dental
<b>Power Tools</b>	<b>Motor Systems</b>	Power Tools, <i>standard</i> Heka Drill, <i>high-speed</i>	Power Tools
<b>Instruments</b>	<b>Screw Removal</b> <b>Miscellaneous Instruments</b> <b>Micro Surgery</b>	S.O.S. Screw Extraction Set Misc.Instruments, Sterilization, Storage Instruments for Micro Surgery	Instruments
<b>Sulcoplasty</b>	<b>Sulcoplasty</b>	Sulcoplasty Set & Instruments	Sulcoplasty

# TTA RAPID®



## More than 150,000 successful surgeries worldwide

Tibial Tuberosity Advancement (TTA) has become a widely popular technique for the surgical correction of cruciate ligament tears in recent years. The introduction of TTA RAPID® has significantly enhanced the original method, making the procedure much simpler and more efficient.


To date, veterinarians globally have performed over 150,000 successful TTA RAPID® surgeries, opting for this improved technique to ensure permanent repair of cruciate ligament tears.



## Now with 59 different cage sizes

With 59 different cage sizes, TTA RAPID® stands out as the most versatile surgical technique designed to repair a cruciate ligament injury.

Ranging from 2mm to 18mm, these cage sizes accommodate all patients, from toy to giant breeds. Our system also includes three different saw guides and five distinct spreaders, providing an unparalleled level of diversity and adaptability that you won't find in any other system.

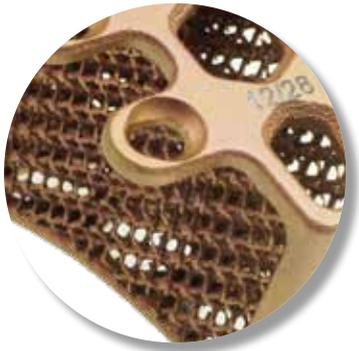

## Rapid Healing + Short Surgery Time


TTA RAPID® implants offer high stability with a less invasive approach. The TTA RAPID® surgery allows for shorter surgery times which means lower risk of infection, less anesthesia, and less costs.

The open sponge Titanium construct allows for rapid bone growth throughout the cage.



## Patella Luxation + CCL Rupture

TTA RAPID® is extremely effective for a patella luxation in combination with a cruciate ligament rupture. The uniquely designed Tibia Tappet allows you to accurately advance the tibial tuberosity and test functionality of the new position before fixating the screws.

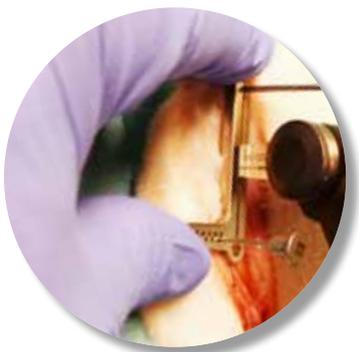


## Minimal Learning Curve

Due to the simplicity of the technique and instruments, a level of comfort can be achieved quickly.



**TTA**<sup>®</sup>  
**RAPID**  
*It's firm, it's safe, it's RAPID.*

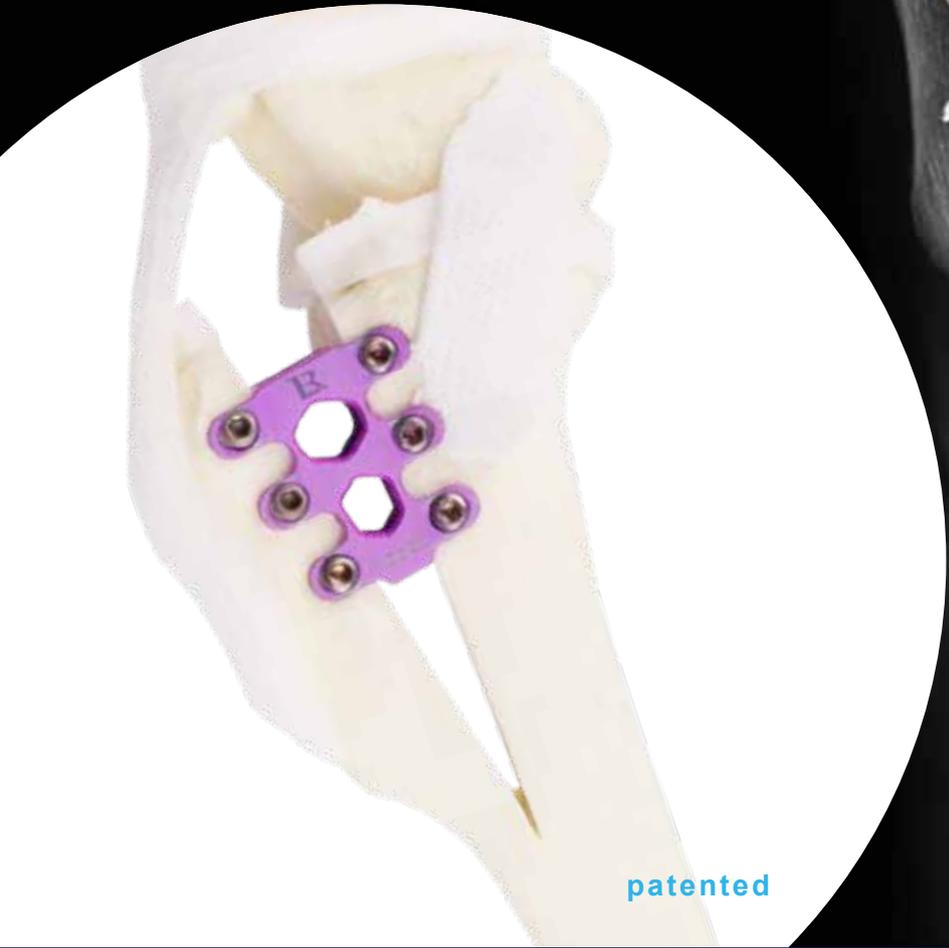

patented



Special Thanks to  
 Dr. Caroline Huisman-Wildeman

**TTA RAPID**<sup>®</sup>



### TTA RAPID®


Tibial Tuberosity Advancement (TTA) as a technique for the surgical management of cranial cruciate ligament insufficiency has gained increasing acceptance and popularity in recent years. As we learn more, efforts are being made to simplify the technique, to make it more user-friendly and overcome some of the pitfalls of the original technique.

Developed in collaboration with Dr. Yves Samoy, University of Ghent, TTA RAPID® is one of the newer developments in both implant technology and technique.

#### The Implant

The manufacture of TTA RAPID® cages has only been made possible with advances in materials and manufacturing technology. The cages are made by an additive manufacturing (AM) 3D printing process known as selective laser sintering (SLS). The process is interesting to watch. Although other materials can be used in the process, TTA RAPID® Cages start life as a very fine, commercially pure titanium powder. A very thin layer of titanium powder is deposited on the working bed of the SLS machine and a modified print head carrying a high intensity laser is used to selectively melt the powder to bond (sinter) regions together. As further layers of powder are applied and the laser sintering process repeated, a solid three dimensional structure begins to form within the 'sand-pit' of metal powder. Electron beam melting (EBM) is a similar procedure that uses an electron beam instead of a laser.

Once the full structure has been created, the cages are separated from the powder and various chemical and other finishing processes are performed to leave the cages in their final, implantable state. Through this process, shapes can be created that would either be impossible to produce using more conventional technologies or cost prohibitive.



In the case of TTA RAPID®, a very porous honeycomb titanium lattice with a modulus similar to that of cancellous bone is generated permitting very rapid bony ingrowth to occur. Titanium is also very biocompatible, MRI compatible and typically needs to be inoculated with 10 times as many infectious

units for an implant associated infection to develop when compared to Stainless Steel.

The lattice found in the TTA Rapid cages is bound on 4 sides by an anatomically shaped, rigid shell of the same material with one side carrying lugs with screw holes in them. With the



lattice, cage and screw lugs being one piece, the cages are very stable in situ.

The constructs are so stable that auxiliary implants such as plates, wires, forks and staples are rarely indicated. This has a number of benefits:

- Reduced morbidity and biological cost that may be associated with the dissection and placement of additional implants.
- Reduced potential for cold conduction with superficially sited metallic implants.
- Fewer additional holes created in the tibial diaphysis which may contribute to crack propagation and failure of the tibial shaft.
- Metals of different electro-potentials are avoided in the same construct. Theoretically this reduces the potential for galvanic corrosion to occur (all components are titanium).
- Simplified inventory management.
- Potential time savings in the placement of implants.

**CAUTION:** TTA RAPID® patients are often subjectively more comfortable in their early post-operative recovery compared to those undergoing other osteotomy surgeries. Nevertheless, TTA RAPID® still involves a major osteotomy, and both appropriate patient selection and appropriate client education for post-operative management are indicated.

## TTA RAPID® TECHNIQUE


### Pre-Operative Planning

#### Calculating the Advancement

Calculating the advancement can be done in different ways (classic TTA template; common tangent technique (Denlser); 2.07 x Tibial plateau Length (Inauen); Ness; ...). However, none of these techniques are perfect. A critical mind is advised when applying those measurements.

#### Using the TTA RAPID® Template

1. Where possible, calibrate the radiograph on the screen to the actual size.
2. Place the template over the radiograph and select the appropriate cage width.
3. Adjust the template position until the cage sits about 3mm below the proximal cortex on its caudal edge. Now measure the thickness of the cranial tibial cortex in the region of the black dot. Note these values as you will need them during surgery: XX / YY / Z

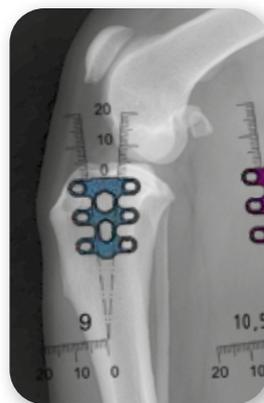

**XX** = Size of Implant from Template

**YY** = Implant Depth (can be measured after the saw cut)

**Z** = Thickness of the cranial tibial cortex in the region of the distal end of the osteotomy.



# TTA RAPID® TECHNIQUE

## Surgery Protocol

The dog is positioned in a dorsal recumbency, with the affected limb suspended from a stand. Make sure that the dog's paws are not fixed too tightly, since the affected limb will be put against the table later in the surgery. Preferably, the joint is thoroughly examined to assess the condition of the menisci and cranial cruciate ligament remnants. Remedial action is taken as necessary.

The TTA RAPID® Procedure is initiated through a medial skin incision.

### Joint Surgery

If performing a lateral arthrotomy, leave about the last centimeter of the joint capsule closest to the tibia open. This allows enough slack to later perform the advancement.

## Sawing the Crista Tibiae

- 1 A 2.5mm pin is placed through the joint capsule at the intersection of the femoral condyle and the tibial plateau. On the lateral side, the pin should start slightly in front of the level of "Gerdy's Tubercle". This pin is used as the proximal fixation of the saw guide.

### Using the Saw Guide



The saw guide is an L-shaped device developed to facilitate the correct positioning of the osteotomy. It was designed to ensure that a sufficiently large cranial fragment is created for screw placement. The vertical arm of the guide has 2.5mm holes placed at strategic points, over a 1mm wide slot. The numbers next to these holes correspond with the size of the cage. This will prevent making a too distal osteotomy. The horizontal arm of the guide is a scale in millimeters. This will prevent making a too caudal osteotomy.



- 2 The guide is dropped over the pin using one of the numbered holes in the vertical arm, corresponding with the size of the cage measured during pre-operative planning.

- 3 A peg is placed into one of the holes in the horizontal arm of the drill guide, selecting the number of millimeters measured during pre-operative planning.
- 4 Press the saw guide against the medial aspect of the tibia with protruding peg forced up against the cranial side of the tibia. Hold it in that position. Correct use of the saw guide will place the osteotomy just caudal to the cranial cortex of the tibia. (As a guide: In a large dog the cortex is approximately 5mm thick and in a small dog approximately 3mm.)

**IMPORTANT: Do not press the horizontal arm against the bone, as this will cause an oblique Osteotomy!**

- 5 Use the saw guide to create the osteotomy. Optionally, a blade can be used to open the fascia/periosteum prior to the osteotomy.



## Opening the Osteotomy

- 1 Depending on the required cage size, different osteotomy spreaders can be used to spread and hold open the osteotomy. Provided this is done carefully and slowly, allowing the bone time to adjust, the hinge is unlikely to fail. This being the most critical point of the surgery, the spreaders should be used with great caution!
- 2 Start with the 3mm spreader held sideways (thinnest part) located at the most proximal part of the osteotomy and gently turn it to spread open the osteotomy. Always turn the spacer downwards to minimize the forces on the fragment. A second spacer/spreader held sideways in the distal region of the osteotomy can be used to maintain the displacement.

**CAUTION: Do not use this second spreader to increase the displacement as this will cause breaking of the cortex!**

Repeat these steps until the required displacement is reached.

- 3 The depth of the osteotomy is measured with a drill depth gauge at the proximal extent of the osteotomy. This measurement is rounded up to select the correct cage Length.

## TTA RAPID® TECHNIQUE

### Fitting the Cage

- 1 The ears of the TTA RAPID® Cage need to be bent using the bending iron. Ears on the caudal side (tibia) should point slightly upwards, while the ears on the cranial side (crista tibiae) should be tilted slightly downwards. Slight under-bending of the caudal ears and slight over-bending of the cranial ears will help compress the osteotomy against the cage.
- 2 Elevate the periosteum from the bone in the region where the cage will be fixed.
- 3 Insert the cage into the osteotomy. Use bone forceps to make sure the ears of the cage are in close contact with the bone.



- 4 Once the cage is in place, check if the height of the cage is correct. This can be done by palpating the proximal tibia with the tip of a small mosquito clamp. You should feel about 3mm of bone above the top of the cage. More bone means a more distal placement of the cage and thus subsequently a more cranial displacement of the tibial tuberosity.
- 5 Large bone forceps can be used to give extra compression on the cage. This step is not essential if the distal cortex is still intact, but will result in a better bone contact with the cage.
- 6 Titanium screws are then inserted into the cage. Start with the most cranial, most proximal screw. The orientation of the screws should be medio-proximal to latero-distal (similar as the orientation of the fork in a standard TTA). The second screw is the caudo-proximal screw. The orientation of this screw is cranio-medio-proximal to caudo-latero-distal ("Away from the joint, away from the osteotomy site"). The rest of the screws are placed in the same fashion starting with the most proximal screws.

Once all screws are inserted, remove the bone forceps and re-tighten all screws.

- 7 Application of Hydroxyapatite Paste inside and underneath the cage will accelerate healing of the osteotomy. Close the fascia where possible.
- 8 Close the wound using standard techniques.



### Aftercare

- 1 Casting/bandaging is generally not required.
- 2 A light dressing can be applied for 3 to 5 days.
- 3 NSAIDs are provided for 3 to 4 weeks.
- 4 With the application of Hydroxyapatite Paste, clinical union can generally be anticipated within 6 weeks.

*Y. Samoy, DVM, PhD and P. Verleyen, DVM  
Department of Medical Imaging and Small Animal Orthopedics  
Faculty of Veterinary Medicine, Ghent University*



**rapid.leibinger.vet**



## STUDIES ABOUT TTA RAPID®

### Comparison of Outcomes Associated with Tibial Plateau Levelling Osteotomy and a Modified Technique for Tibial Tuberosity Advancement for the Treatment of Cranial Cruciate Ligament Disease in Dogs: A Randomized Clinical Study

University of Lyon, VetAgro Sup, Marcy l'Etoile, France  
Véronique Livet, Arnaud Baldinger, Éric Viguier, Mathieu Taroni, Mathieu Harel, Claude Carozzo, Thibaut Cachon; VCOT 2019

### TTA RAPID: Description of the Technique and Short Term Clinical Trial Results of the First 50 Cases

Ghent University, Faculty of Veterinary Medicine, Department of Veterinary Medical Imaging and Small Animal Orthopaedics  
Yves Samoy, DVM, PhD, Geert Verhoeven, DVM, PhD, Diplomate ECVS, Tim Bosmans, DVM, PhD, Elke Van der Vekens, DVM, Diplomate ECVI, Evelien de Bakker, DVM, PhD, Piet Verleyen, DVM and Bernadette Van Ryssen, Prof, DVM, PhD; Vet Surg 2014

### Tibial tuberosity advancement in small-breed dogs using TTA RAPID implants. Complications and outcome

Evidensia Strömsholm Small Animal Referral Hospital, Sweden; Dyall B A R, DVM, Spec SWE. Schmökel H, DVM, DECVS, PHD; 2016

### TTA RAPID in the treatment of the canine cruciate deficient stifle: short- and medium-term outcome

S. J. Butterworth & D. M. Kydd, Weighbridge Referral Centre & Kydd & Kydd Vets; Journal of Small Animal Practice 2017

### TTA RAPID for treatment of cranial cruciate ligament injuries in dogs. Clinical results 50 cases

Kydd and Kydd Veterinary Health Centre, Wimbledon  
David M Kydd BVetMed CertVR CertSAO MRCVS; Orthopaedic News from Kydd & Kydd 2014

### Postoperative infection with a multiresistant Staphylococcus aureus (MRSA) in a Bernese mountain dog with a rupture of the cranial cruciate ligament

Ghent University, Faculty of Veterinary Medicine, Department of Veterinary Medical Imaging and Small Animal Orthopaedics; F. Vandael, E. de Bakker, D. Paepe, L. Mosselmans, Y. Samoy, G. Verhoeven, B. Van Ryssen; Flemish Veterinary Journal, 2015, 84

### TTA RAPID: an interesting alternative operation method of an injured cranial cruciate ligament

Lecznica Weterynaryjna Arwet w Wieliczce; lek. wet. Rafał Korta; VETERYNARIA W PRAKTYCE 2014

### Bone Regeneration in Critical-Sized Bone Defects Treated with Additively Manufactured Porous Metallic Biomaterials: The Effects of Inelastic Mechanical Properties

M. Koolen, S.A. Yavari, K. Lietaert, R. Wauthle, A.A. Zadpoor, H. Weinans; Universities of Utrecht & Delft, 3D Systems Healthcare; MDPI Journals (Materials) 2020

### TTA RAPID® with porous structure stimulates bone ingrowth

"TTA RAPID is made from pure titanium using innovative additive manufacturing (3D printing) technologies that allow to create complex geometries like porous structures.

These porous structures stimulate bone ingrowth through the open porosities, have an improved fixation thanks to the high roughness and corresponding coefficient of friction, and have, in addition, a lower stiffness and thus avoid stress-shielding.

The mechanical and clinical performance of the dodecahedron unit cell – also used in TTA RAPID – has been reported in literature, showing superior dynamical properties<sup>1</sup> and bone regeneration<sup>2</sup> compared to standard Ti-6Al-4V porous structures. These research-based innovations are the cornerstone of TTA RAPID, leading to over 80,000 TTA RAPID cages successfully implanted since 2011."

<sup>1</sup> Wauthle et al., Revival of pure titanium for dynamically loaded porous implants using additive manufacturing. Mater. Sci. Eng. C Mater. Biol. Appl. 2015, 54, 94–100.

<sup>2</sup> Koolen et al., Bone Regeneration in Critical-Sized Bone Defects Treated with Additively Manufactured Porous Metallic Biomaterials: The Effects of Inelastic Mechanical Properties. Materials 2020, 13, 1992.

**NEW**

**TTA RAPID® Giant Set**

**Perfect for giant dog breeds!**

Contains the big cage sizes 13.5mm and 15mm with depths ranging from 19 to 28mm, as well as the **new giant cage sizes 16.5mm and 18mm** with depths from 22mm up to 31mm.

**TTA RAPID® Giant Set**

- Contains:
- Sterilization Tray with Lid
- 3x 2.4mm Screws of each length (6-40mm, 54 pcs. total)
- 2x 2.7mm Screws of each length (10-50mm, 36 pcs. total)
- 1 Cage of each size from 13.5 to 18mm (16 cages total)

Set with LeiStar Screws

**132-6200-00**

Tray without contents

**132-6200-10**



**TTA RAPID® Premium Set**

- Contains:
- Sterilization Tray with Lid
- 5x 2.4mm Screws of each length (6-40mm, 90 pcs. total)
- 1 Cage of each size from 3 to 12mm
- Plus: 1 additional cage each of the short and very short cages (42 cages total)

Set with LeiStar Screws

**132-6012-00**

Set with Hexagonal Screws

**132-6002-00**

Tray without contents

**132-5000-00/A**





TTA RAPID Starter Sets

TTA RAPID Starter Sets I, II, III

**TTA RAPID® Starter Split Set I**

Contains:  
Sterilization Tray with Lid  
5x 2.4mm Screws of each length  
(6-40mm, 90 pcs. total)  
1 Cage of each size from 3 to 12mm  
(28 cages total)

Set with LeiStar Screws

**132-6013-00**

Set with Hexagonal Screws

**132-6003-00**

Tray without contents

**132-5000-00/A**



**TTA RAPID® Starter Set II**

Contains:  
Sterilization Tray with Lid  
5x 2.4mm Screws of each length  
(6-40mm, 90 pcs. total)  
1 Cage of each size from 6mm to 10.5mm  
Plus: 1 additional cage each of the short and very short  
cages (24 cages total)

Set with LeiStar Screws

**132-6014-00**

Set with Hexagonal Screws

**132-6004-00**

Tray without contents

**132-5000-00/A**



**TTA RAPID® Starter Set III**

Contains:  
Sterilization Tray with Lid  
5 pcs. 2.4mm Screws of each length  
(6-40mm, 90 pcs. total)  
1 Cage of each size from 6 to 10.5mm  
(16 Cages total)

Set with LeiStar Screws


**132-6015-00**

Set with Hexagonal Screws

**132-6005-00**

Tray without contents

**132-5000-00/A**

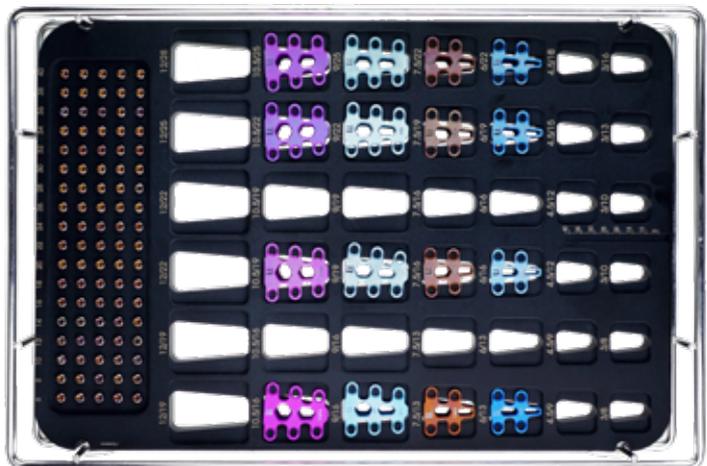

**TTA RAPID® Starter Set IV**

Contains:

Sterilization Tray with Lid

5 pcs. 2.4mm Screws of each length  
(6-40mm, 90 pcs. total)

1 Cage of each size from 6 to 10.5mm,  
not including the longest versions  
(12 Cages total)

Set with LeiStar Screws

**132-6016-00**

Set with Hexagonal Screws

**132-6006-00**

Tray without contents

**132-5000-00/A**



**TTA RAPID® Instrument Kit**

Contains:

Sterilization Tray

Petite Saw Guide (not Tiny) + K-Wire

Standard Sawguide + K-Wire

1 Pin

Lever-Spreader 3/9 + 6/12

Twist Drill 1.8

Depth Gauge

Screwdriver Handle

Screw Driver Shaft 2.4 + Holding Sleeve

Drill Guide

Plate Holding Forceps

Set with LeiStar (Holding Sleeve not included)


**132-6010-00**

Set with Hex

**132-6000-10**

Tray without contents

**132-5000-10/A**

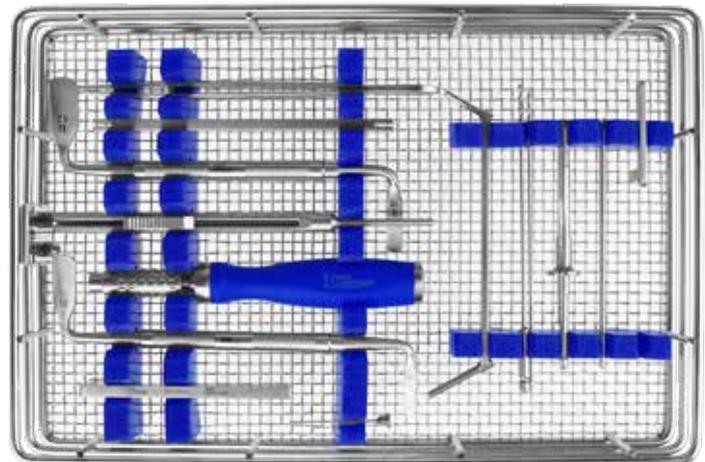

**Sterilization Container**

See Sterilization Containers for Implants and Instruments Trays on **Page 204.**



## TTA RAPID® TINY SYSTEM

### TTA RAPID® Tiny Set

#### Specially developed for tiny patients

The TTA RAPID® Tiny System is specifically designed for our smallest companions, including cats, toy breed dogs, and dogs with short legs. Engineered to address the delicate anatomical nuances of these patients, the set features 1.5mm and 2.0mm cages and screws. Accompanying instrumentation includes a "tiny" sawguide and spreader, allowing short osteotomies and ensuring meticulous surgical precision for the tiniest patients.



### TTA RAPID® Tiny Set

Contains:

- 1 Sterilization Tray with Lid
- 1 of each TTA RAPID® Tiny Cage (12 total)
- 1 of each 2, 3 & 4mm Patella Spacer (6 total)
- 1 Rapid Luxation Plate "Petite"
- 5 of each 1.5mm Screw (6-20mm, 40 total)
- 5 of each 2.0mm Screw (6-26mm, 55 total)
- 1 Tibia Tappet Petite
- 1 Plate Holding Forceps
- 1 Tiny Sawguide with Pin & K-Wire
- 1 Depth Gauge
- 2 Drills (1.1 & 1.5mm)
- 2 Screw Driver Shafts (T6 & T8)
- 1 Screwdriver Handle
- 1 Drill Guide

Set with LeiStar Screws

**132-6500-00**

Tray without contents

**132-6500-10**

### Complete Solution for CrCL + Patella Luxation

The TTA RAPID® Tiny Set includes Patella Spacers, a RAPID Luxation Plate, and the essential instruments to treat a cruciate ligament rupture and a concomitant Patella Luxation in one surgery.


Learn more about this procedure on **Page 21**.



**NEW**

### Suture Holes for More Rotational Stability


The TTA RAPID® Tiny cages now feature a suture hole that allows passing a suture material through the cage and a bone anchor in the distal femur.

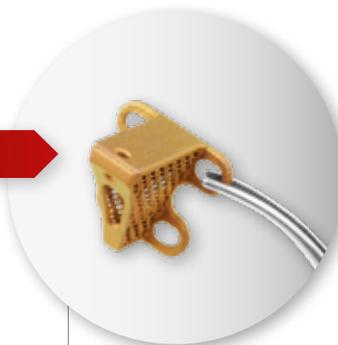

TTA RAPID® Tiny Cages

Titanium

	Product Code	Size in mm (width/depth)	Screw Size
	132-0152-06	2/06	for 1.5 screws
	132-0152-08	2/08	for 1.5 screws
	132-0152-10	2/10	for 1.5 screws
	132-0153-07	3/07	for 1.5 / 2.0 screws
	132-0153-09	3/09	for 1.5 / 2.0 screws
	132-0153-11	3/11	for 1.5 / 2.0 screws
	132-0245-08	4.5/08	for 2.0 screws
	132-0245-10	4.5/10	for 2.0 screws
	132-0245-12	4.5/12	for 2.0 screws
	132-0026-09	6/09	for 2.0 screws
	132-0026-11	6/11	for 2.0 screws
	132-0026-13	6/13	for 2.0 screws



**NEW**


**Suture Holes for More Rotational Stability**

The TTA RAPID® Tiny cages now feature a hole that allows passing a suture material through the cage and a bone anchor in the distal femur to temporarily increase the post-operative rotational stability in highly unstable stifle joints with a CrCL rupture and pivot shift.

TTA RAPID® Cages

Titanium

	Product Code	Size in mm (width/depth)	Screw Size
	132-0023-08	3/08 (petite)	for 2.0 screws
	132-0023-10	3/10 (petite)	for 2.0 screws
	132-0023-13	3/13 (petite)	for 2.0 screws
	132-0003-08	3/08	for 2.4 screws
	132-0003-10	3/10	for 2.4 screws
	132-0003-13	3/13	for 2.4 screws
	132-0003-16	3/16	for 2.4 screws
	132-0045-09	4.5/09	for 2.4 screws
	132-0045-12	4.5/12	for 2.4 screws
	132-0045-15	4.5/15	for 2.4 screws
	132-0045-18	4.5/18	for 2.4 screws
	132-0006-13	6/13	for 2.4 screws
	132-0006-16	6/16	for 2.4 screws
	132-0006-19	6/19	for 2.4 screws
	132-0006-22	6/22	for 2.4 screws
		132-0075-13	7.5/13
132-0075-16		7.5/16	for 2.4 screws
132-0075-19		7.5/19	for 2.4 screws
132-0075-22		7.5/22	for 2.4 screws

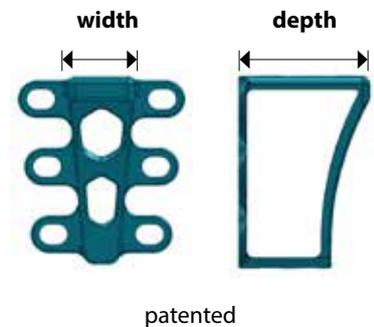



## TTA RAPID Giant Cages



### TTA RAPID® Cages

Titanium

Product Code	Size in mm (width/depth)	Screw Size
132-0009-16	9/16	for 2.4 screws
132-0009-19	9/19	for 2.4 screws
132-0009-22	9/22	for 2.4 screws
132-0009-25	9/25	for 2.4 screws
132-0105-16	10.5/16	for 2.4 screws
132-0105-19	10.5/19	for 2.4 screws
132-0105-22	10.5/22	for 2.4 screws
132-0105-25	10.5/25	for 2.4 screws
132-0012-19	12/19	for 2.4 screws
132-0012-22	12/22	for 2.4 screws
132-0012-25	12/25	for 2.4 screws
132-0012-28	12/28	for 2.4 screws



### TTA RAPID® Giant Cages

Titanium

Product Code	Size in mm (width/depth)	Screw Size
132-0135-19	13.5/19	for 2.4 / 2.7 screws
132-0135-22	13.5/22	for 2.4 / 2.7 screws
132-0135-25	13.5/25	for 2.4 / 2.7 screws
132-0135-28	13.5/28	for 2.4 / 2.7 screws
132-0015-19	15/19	for 2.4 / 2.7 screws
132-0015-22	15/22	for 2.4 / 2.7 screws
132-0015-25	15/25	for 2.4 / 2.7 screws
132-0015-28	15/28	for 2.4 / 2.7 screws
132-0165-22	16.5/22	for 2.4 / 2.7 screws
132-0165-25	16.5/25	for 2.4 / 2.7 screws
132-0165-28	16.5/28	for 2.4 / 2.7 screws
132-0165-31	16.5/31	for 2.4 / 2.7 screws
132-0018-22	18/22	for 2.4 / 2.7 screws
132-0018-25	18/25	for 2.4 / 2.7 screws
132-0018-28	18/28	for 2.4 / 2.7 screws
132-0018-31	18/31	for 2.4 / 2.7 screws



NEW



NEW



### 1.5 Cortical Screws, Titanium

LeiStar head, self tapping, with three flute cutting edge



Length (mm)	LeiStar
6	245-515-06
7	245-515-07
8	245-515-08
9	245-515-09
10	245-515-10
12	245-515-12
14	245-515-14
16	245-515-16
18	245-515-18
20	245-515-20

See more screw lengths on **Page 126.**

Screw Racks on **Page 198.**

### 2.4 Cortical Screws, Titanium

Hexagonal or LeiStar Head, self tapping, with three flute cutting edge



Length (mm)	Hexagonal (Standard)	LeiStar (Standard)
6	245-224-06	245-524-06
8	245-224-08	245-524-08
10	245-224-10	245-524-10
12	245-224-12	245-524-12
14	245-224-14	245-524-14
16	245-224-16	245-524-16
18	245-224-18	245-524-18
20	245-224-20	245-524-20
22	245-224-22	245-524-22
24	245-224-24	245-524-24
26	245-224-26	245-524-26
28	245-224-28	245-524-28
30	245-224-30	245-524-30
32	245-224-32	245-524-32
34	245-224-34	245-524-34
36	245-224-36	245-524-36
38	245-224-38	245-524-38
40	245-224-40	245-524-40

### 2.0 Cortical Screws, Titanium

Hexagonal or LeiStar head, self tapping, with three flute cutting edge



Length (mm)	Hexagonal	LeiStar
6	245-220-06	245-520-06
8	245-220-08	245-520-08
10	245-220-10	245-520-10
12	245-220-12	245-520-12
14	245-220-14	245-520-14
16	245-220-16	245-520-16
18	245-220-18	245-520-18
20	245-220-20	245-520-20
22	245-220-22	245-520-22
24	245-220-24	245-520-24
26	245-220-26	245-520-26
28	245-220-28	245-520-28
30	245-220-30	245-520-30

### 2.7 Cortical Screws, Titanium

Hexagonal or LeiStar Head, self tapping, with three flute cutting edge




Length (mm)	LeiStar (Standard)
10	245-527-10
12	245-527-12
14	245-527-14
16	245-527-16
18	245-527-18
20	245-527-20
22	245-527-22
24	245-527-24
26	245-527-26
28	245-527-28
30	245-527-30
32	245-527-32
34	245-527-34
36	245-527-36
38	245-527-38
40	245-527-40
45	245-527-45
50	245-527-50



## TTA RAPID® & RAPID PATELLA LUXATION SYSTEM

### Correction of a Patella Luxation during a TTA RAPID® Surgery

This technique is suitable for dogs suffering from patella luxation with a simultaneous cruciate ligament tear, a partial cruciate ligament tear, or when a cruciate ligament tear is imminent.




[tta.leibinger.net](http://tta.leibinger.net)

## TTA + PATELLA LUXATION (TTTA)

**Dr. Hugo Schmökel**

When a dog suffers from a cranial cruciate ligament rupture with a simultaneous patellar luxation, this can be addressed with a modified TTA RAPID® procedure. Prior to the TTA RAPID® surgery itself, it should be determined if the dog would benefit from a trochleoplasty. If so, this should be performed before the actual TTA RAPID® procedure<sup>1</sup>.

The osteotomy used for the TTA RAPID® procedure can also be used to achieve a medial or lateral tibial tuberosity transposition (TTT), depending on the kind of patellar luxation. The further described procedure focuses on a lateralization of the crest, needed for the correction of a medial patellar luxation.



After performing the osteotomy, the appropriate cage is inserted into the osteotomy and all of the caudal screws are inserted in the tibia (*Image 1*). Take care to choose a cage that has a bigger medio-lateral length than measured after the osteotomy, as both cortices of the transposed crest need to be supported! Usually, the longest cage is advised.

Consecutively, the tibial crest is slightly advanced, so that it can be moved laterally with the tibia tapet instrument (*Image 2*).



Be very careful performing this and restrict the advancement to the absolute minimum to avoid crest avulsion. Once the desired position is reached, a corresponding washer is placed between the crista tibiae and the ears of the cage (*Image 3*).

If the transposition is sufficient to prevent dislocation of the patella, the remaining screws are inserted and the operation finished as described (*Images 4 and 5*).

In case of a lateral luxation, the tibial crest is shifted medially in a similar manner after fixating the cranial part of the cage in the tibial crest.

1. Samoy Y, Verhoeven G, Bosmans T, Van der Vekens E, de Bakker E, Verleyen P, et al. TTA RAPID: Description of the Technique and Short Term Clinical Trial Results of the First 50 Cases. *Vet Surg.* 2014;n/a-n/a.

**Patella Luxation Spacers**

For RAPID LUXATION and TTA RAPID, Titanium



Product Code	Specifications	For Cage Sizes
132-8030-01L	1 mm height, 2 holes, left	Tiny / Petite
132-8030-01R	1 mm height, 2 holes, right	Tiny / Petite
132-8030-02L	2 mm height, 2 holes, left	Tiny / Petite
132-8030-02R	2 mm height, 2 holes, right	Tiny / Petite
132-8030-03L	3 mm height, 2 holes, left	Tiny / Petite
132-8030-03R	3 mm height, 2 holes, right	Tiny / Petite
132-8030-04L	4 mm height, 2 holes, left	Tiny / Petite
132-8030-04R	4 mm height, 2 holes, right	Tiny / Petite
132-8020-02L	2 mm height, 2 holes, left	3 - 7,5 mm
132-8020-02R	2 mm height, 2 holes, right	3 - 7,5 mm
132-8020-03L	3 mm height, 2 holes, left	3 - 7,5 mm
132-8020-03R	3 mm height, 2 holes, right	3 - 7,5 mm
132-8020-04L	4 mm height, 2 holes, left	3 - 7,5 mm
132-8020-04R	4 mm height, 2 holes, right	3 - 7,5 mm
132-8010-02L	2 mm height, 3 holes, left	9 - 15 mm
132-8010-02R	2 mm height, 3 holes, right	9 - 15 mm
132-8010-04L	4 mm height, 3 holes, left	9 - 15 mm
132-8010-04R	4 mm height, 3 holes, right	9 - 15 mm
132-8010-06L	6 mm height, 3 holes, left	9 - 15 mm
132-8010-06R	6 mm height, 3 holes, right	9 - 15 mm

**Tibia Tappet**

For inserting Patella Luxation Spacers.



Product Code	Description
132-4071-00	Petite / Tiny 2.0 mm
132-4070-00	Standard 2.4 mm



**Patella Saw**

With standard sawblade, incl. Allen Wrench 1.5mm

**23-1005-90**

Replacement Saw Blade

**23-1005-20**





# TTA RAPID® & RAPID LUXATION SYSTEM INSTRUMENTS

## TTA RAPID® Spreader


With tensioning and fixation screw

Product Code	Description
132-4080-12	12 cm (Tiny)
132-4080-16	16 cm (Standard)



## TTA RAPID® Lever-Spreader

Product Code	Description
132-4000-13	3 mm & 9 mm (Tiny)
132-4010-13	6 mm & 12 mm
132-4015-13	13.5 mm & 15 mm

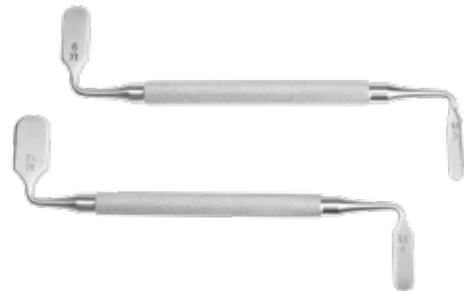

## TTA RAPID® Saw Guide


Product Code	Description
132-4042-00	For Tiny cage sizes 2 - 6 mm
132-4041-00	For cage sizes 3 - 4.5 mm
132-4040-00	For cage sizes 6 - 15 mm



## TTA RAPID® Saw Guide Pin

Ø 1.0mm

132-4030-10



### Saw Blades

See saw blades on **Page 190**.



### Calibration Ball

See Radiography Calibration Ball on **Page 81**.

## OTHER ESSENTIAL INSTRUMENTS

### Depth Gauge



Product Code	Description	Compatibility
164-1520-20	150mm in length, scale up to 40mm	for 1.5/2.0/2.4 mm screws
164-2735-60	150mm in length, scale up to 60mm	for 2.4/2.7/3.5 mm screws

### Drill Guide

Product Code	Size (mm)	Length (mm)
164-0070-20	1.1/1.5	100 mm
164-0070-18	1.5/1.8	100 mm
164-0070-27	2.0/2.7	100 mm
164-0070-35	2.5/3.5	100 mm



### K- Wires, Single Trocar

Product Code	Description
144-1015-10	1.5 mm x 100 mm
144-1025-10	2.5 mm x 100 mm



See more K-Wires on [Page 136](#).

### Plate Holding Forceps

90 mm, curved

164-0050-09



### Plate Holding Forceps

160 mm, angulated

164-0050-16



### Bone Holding Forceps

21,5 cm - with spin lock

128-0525-21



### TTA Bending Iron

120 mm

132-4020-00





## Twist Drill

## Screwdriver Shaft

## Screwdriver Handle

### Twist Drill



Product Code	Ø (mm)	for Screw Ø (mm)	Length (mm)	Connection
148-0080-11	1.1	for 1.5 screws	60	round shaft
148-0080-15	1.5	for 2.0 screws	70/30	round shaft
148-0080-18	1.8	for 2.4 screws	125/25	round shaft
148-0080-20	2.0	for 2.7 screws	85/70	round shaft



Product Code	Ø (mm)	for Screw Ø (mm)	Length (mm)	Connection
148-0081-11	1.1	for 1.5 screws	60	AO QC
148-0081-15	1.5	for 2.0 screws	85/60	AO QC
148-0081-18	1.8	for 2.4 screws	125/25	AO QC
148-0081-20	2.0	for 2.7 screws	100/75	AO QC

See more Twist Drills on **Page 199**.

### Screwdriver Shaft LeiStar

AO connection, self-holding  
(no Holding Sleeve needed)



Product Code	Description
128-1520-15	T6, for 1.5 mm Screws, 60 mm in length
128-1520-20	T8, for 2.0 / 2.4 mm screws, 60 mm in length
128-2024-08	T8, for 2.0 / 2.4 mm screws, 100 mm in length
128-2735-10	T10, for 2.7 / 3.5 mm screws, 100 mm in length

### Screwdriver Shaft Hexagonal

AO connection (Holding Sleeve recommended)



Product Code	Description
128-0900-15	for 2.0 mm Screws, 100 mm long
128-0900-20	for 2.4 mm Screws, 100 mm long

More Screwdriver Shafts on **Page 200**.

### Holding Sleeve

for Hexagonal Screwdriver Shafts

Product Code	Size
128-0940-24	2.0 / 2.4 mm




### Screwdriver Handle

Silicone, AO-Connection  
sterilizable up to 134°C / 273°F



247-0103-00

# RAPID LUXATION

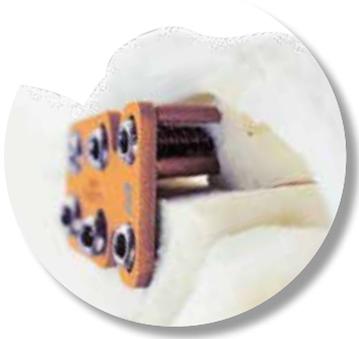

## Patella Correction – Safe And Simple

Patella Luxations are frequently seen in dogs and cats. In the past, correcting these could prove to be challenging, but RAPID LUXATION has simplified the technique and instrumentation.



## Testing The Stifle During The Surgery

The uniquely designed Tibia Tappet allows you to move the tibial tuberosity very accurately and test the functionality of the new position during the surgery before placing the screws.

Once the desired position is reached, it can be securely fixed with the patella spacer and screws.



## Secure Construction

The screws securely fix the plate and spacer together and do not allow movement of the bone, which is essential for quick bone growth.

If you realize a reoperation is necessary post-operatively, you only need to replace the spacer with another size.



## Three Different Sizes


The RAPID LUXATION Patella Plates are available in three different sizes: Petite/Tiny (2.0mm), Medium (2.4mm) and Large (2.4mm).



## Compatible With TTA RAPID®

RAPID LUXATION is compatible with TTA RAPID® since both techniques use identical instrumentation (sawguide, tibia tappet, etc.), screws and patella spacers.

# RAPID LUXATION PLATING SYSTEM

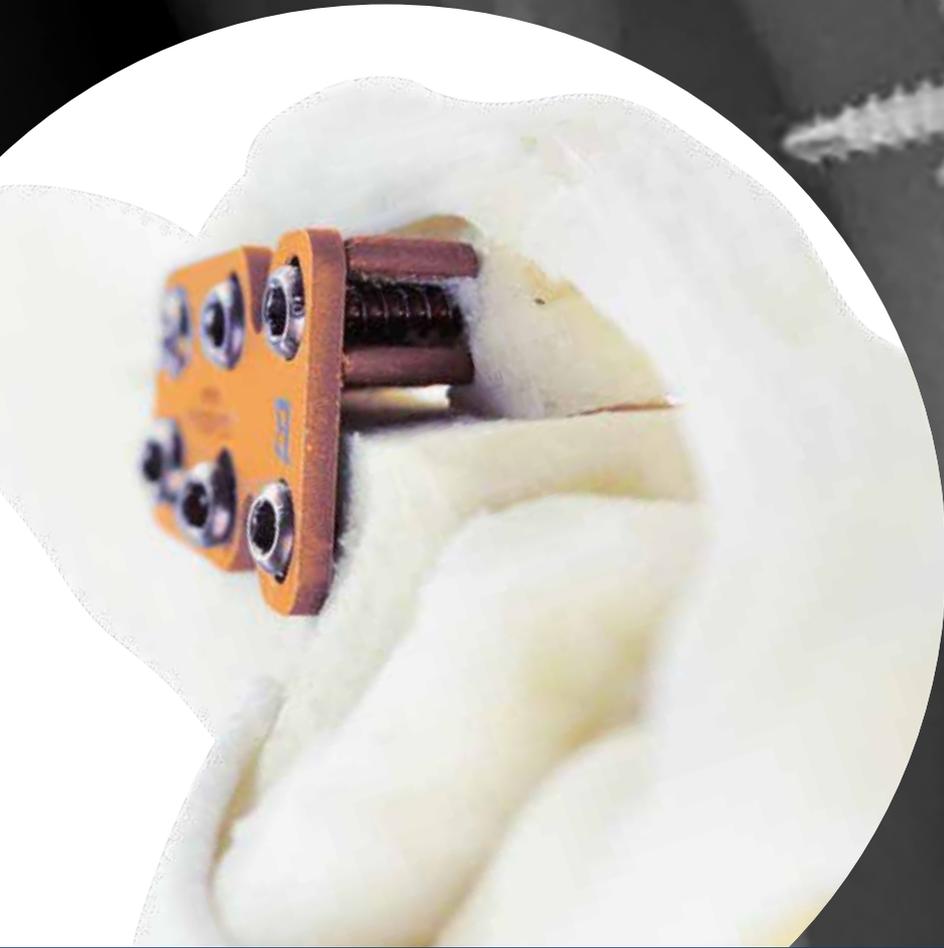

Special Thanks to  
Emile Pickee

## RAPID LUXATION

**R** RITA  
LEIBINGER  
MEDICAL

## RAPID LUXATION SURGERY PROTOCOL

### Placement of the Patient

The dog is positioned in a dorsal recumbency, with the affected limb suspended from a stand. Make sure that the dog's paws are not fixed too tightly, as the affected limb will later be placed against the table during the surgery.

The RAPID Luxation procedure is initiated through a medial skin incision.

### Using the Saw Guide



The saw guide is an L-shaped device developed to facilitate the correct positioning of the osteotomy. It was designed to ensure that a sufficiently large cranial fragment is created for screw placement. The vertical arm of

the guide has 2.5mm holes placed at strategic points, over a 1mm wide slot, with markings derived from the TTA RAPID® technique, making it equally suitable for the RAPID Luxation technique to prevent overly distal osteotomies. The horizontal arm of the guide includes a millimeter scale, preventing overly caudal osteotomies and ensuring accurate alignment during surgery.

### Making the Osteotomy

- 1 A 2.5mm pin is placed through the joint capsule at the intersection of the femoral condyle and the tibial plateau. On the lateral side, the pin should start slightly in front of the level of "Gerdy's Tubercle". This pin is used as the proximal fixation of the saw guide.



- 2 The saw guide is dropped over the pin using one of the numbered holes in the vertical arm. The selected number should ensure that the osteotomy ends just below the Tibial Tuberosity.
- 3 A peg is placed into one of the holes in the horizontal arm of the drill guide, selecting the cortical thickness in millimeters measured during pre-operative planning.
- 4 Press the saw guide against the medial aspect of the tibia with protruding peg forced up against the cranial side of the tibia. Hold it in that position. Correct use of the saw guide will place the osteotomy just caudal to the cranial cortex of the tibia. (As a guide: In a large dog the cortex is approximately 5mm thick and in a small dog approximately 3mm.)

**IMPORTANT: Do not press the horizontal arm against the bone, as this will cause an oblique Osteotomy!**



- 5 Use an oscillating saw to create the osteotomy. Optionally, a blade can be used to open the fascia/periosteum prior to the osteotomy.

### Placing the Implants

In the following, a medial Patella Luxation (PL) is described. In a lateral PL, place the implants in the lateral/medial opposite site.



- 1 The RAPID Luxation Plate is placed on the tibia. The osteotomy should be in the middle of the RAPID Luxation Plate. The plate is then screwed on the caudal side of the tibia (for a medial PL) (Note: Place screws on the cranial side for a lateral patella luxation.)



- 2 The RAPID Luxation Tibia Tappet is inserted on the cranial screw holes (top and centre screw hole for the 3-hole plates) of the RAPID Luxation Plate.



- 3 Then the tappet can be rotated, it fixates itself in the screw holes of the RAPID Luxation Plate and transposes the tibia crest to the lateral side. The scale (in mm) on the top of the instruments shows exactly how far the tibia crest is transposed.



- 4 During transposition using the tappet, the stifle can be flexed and extended to check if there is perfect alignment of the patella and if the patella stays in place. If the alignment is not optimal, the transposition can be further increased.



- 5 Once the desired position is achieved, insert the RAPID Luxation Spacer between the plate and the bone. The tappet may then be removed.



- 6 Insert the remaining screws to secure the plate and spacer. Close the fascia where possible. Close the wound according to standard procedure.





**RAPID Luxation Set**

**RAPID Luxation Set**

Contains:

- Sterilization Tray with Lid
- 3 of each 2.0mm Screw (6-20mm)  
(24 pcs. total)
- 3 of each 2.4mm Screw (6-40mm)  
(54 pcs. total)
- 1 of each Rapid Luxation Plate  
(3 pcs. total)
- 1 of each Patella Spacer (18 pcs. total)
- Large Sawguide with Pin & K-Wire
- Petite Sawguide with Pin & K-Wire
- Tibia Tappet Petite
- Tibia Tappet Standard
- Screwdriver Handle
- Screw Driver Shaft 2.4/2.0 or T8
- Holding Sleeve (Hexagonal Set only)
- Plate Holding Forceps
- Depth Gauge
- Drill Guide
- Drills 1.5 + 1.8

Set with Hexagonal Screws

**132-8000-00**

Set with LeiStar Screws

**132-8000-01**

Tray without contents

**132-8000-10**



**luxation.leibinger.vet**



**EXPLORE NOW**

**Sulcoplasty Set & Instruments**


See our Sulcoplasty Set and our range of sulcoplasty instruments on **Page 212** .

**RAPID LUXATION VIDEO**

Watch the animation video of the RAPID Patella Luxation Technique.

Visit our website:

**[www.leibinger.vet/rapid-patella-luxation/rapid-patella-luxation-technique](http://www.leibinger.vet/rapid-patella-luxation/rapid-patella-luxation-technique)**

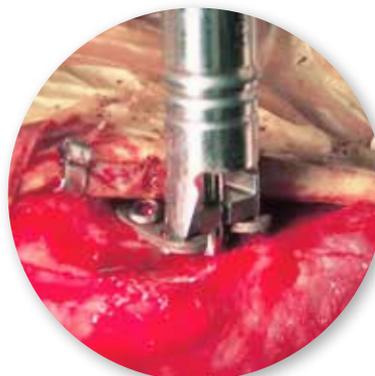

**Luxation Plate**

6-hole, 1.5 mm thick, with gliding holes, for 2.4 mm screws, Titanium

132-8200-01



**Spacer**



Product Code	Spacer left
132-8010-02L	2 mm height, 3 holes, left
132-8010-04L	4 mm height, 3 holes, left
132-8010-06L	6 mm height, 3 holes, left



Product Code	Spacer right
132-8010-02R	2 mm height, 3 holes, right
132-8010-04R	4 mm height, 3 holes, right
132-8010-06R	6 mm height, 3 holes, right

**Luxation Plate**

4-hole, 1 mm thick, with gliding holes for 2.4 mm screws, Titanium

132-8200-02



**Spacer**



Product Code	Spacer left
132-8020-02L	2 mm height, 2 holes, left
132-8020-03L	3 mm height, 2 holes, left
132-8020-04L	4 mm height, 2 holes, left



Product Code	Spacer right
132-8020-02R	2 mm height, 2 holes, right
132-8020-03R	3 mm height, 2 holes, right
132-8020-04R	4 mm height, 2 holes, right

**Luxation Plate Petite**

4-hole, 1 mm thick, with gliding holes for 2.0 mm screws, Titanium

132-8200-03



**Spacer**



Product Code	Spacer left
132-8030-01L	1 mm height, 2 holes, left
132-8030-02L	2 mm height, 2 holes, left
132-8030-03L	3 mm height, 2 holes, left
132-8030-04L	4 mm height, 2 holes, left




Product Code	Spacer right
132-8030-01R	1 mm height, 2 holes, right
132-8030-02R	2 mm height, 2 holes, right
132-8030-03R	3 mm height, 2 holes, right
132-8030-04R	4 mm height, 2 holes, right



**RAPID Luxation Screws**


**Screws for RAPID Luxation**

**2.0 Self-tapping Screws, Titanium**  
Hexagonal or LeiStar head, self tapping, with three flute cutting edge



Length (mm)	Hexagonal (Petite)	LeiStar (Petite)
5		245-520-05
6	245-220-06	245-520-06
7		245-520-07
8	245-220-08	245-520-08
9		245-520-09
10	245-220-10	245-520-10
12	245-220-12	245-520-12
14	245-220-14	245-520-14
16	245-220-16	245-520-16
18	245-220-18	245-520-18
20	245-220-20	245-520-20
22	245-220-22	245-520-22
24	245-220-24	245-520-24
26	245-220-26	245-520-26
28	245-220-28	245-520-28
30	245-220-30	245-520-30

**2.4 Self-tapping Screws, Titanium**  
Hexagonal or LeiStar head, self tapping, with three flute cutting edge



Length (mm)	Hexagonal (Standard)	LeiStar (Standard)
6	245-224-06	245-524-06
8	245-224-08	245-524-08
10	245-224-10	245-524-10
12	245-224-12	245-524-12
14	245-224-14	245-524-14
16	245-224-16	245-524-16
18	245-224-18	245-524-18
20	245-224-20	245-524-20
22	245-224-22	245-524-22
24	245-224-24	245-524-24
26	245-224-26	245-524-26
28	245-224-28	245-524-28
30	245-224-30	245-524-30
32	245-224-32	245-524-32
34	245-224-34	245-524-34
36	245-224-36	245-524-36
38	245-224-38	245-524-38
40	245-224-40	245-524-40

See more screw lengths on **Page 126**.

Screw Racks on **Page 198**.

LEARN FROM THE BEST

**WORKSHOPS & ONLINE COURSES**

Learn the TTA RAPID® & Patella Luxation Technique online or in one of our workshops.

**academy.leibinger.vet**



Online Shop

**veterinary.shop**

Tibia Tappet

Patella Saw

RAPID Luxation Saw Guide

Depth Gauge

**Tibia Tappet**

For inserting Patella  
Luxation Spacers



Product Code	Description
132-4071-00	Petite / Tiny 2.0 mm
132-4070-00	Standard 2.4 mm



**Patella Saw**

With standard sawblade, incl. Allen Wrench 1.5mm

**23-1005-90**

Replacement Saw Blade

**23-1005-20**



**RAPID LUXATION Saw Guide**

Product Code	Description
132-4040-00	for plates 132-8200-01 & -02
132-4041-00	for plates 132-8200-02 & -03
132-4042-00	for Petite plates 132-8200-03



**TTA RAPID® Saw Guide Pin**

Ø 1.0mm

**132-4030-10**



**Depth Gauge**



Product Code	Description	Compatibility
164-1520-20	150mm in length, scale up to 40mm	for 1.5/2.0/2.4 mm screws
164-2735-60	150mm in length, scale up to 60mm	for 2.4/2.7/3.5 mm screws

**Plate Holding Forceps**

90 mm, curved

**164-0050-09**





### Drill Guide

Product Code	Size (mm)	Length (mm)
164-0070-18	1.5/1.8	100 mm



### K- Wires, Single Trocar

Product Code	Description
144-1015-10	1.5 mm x 100 mm
144-1025-10	2.5 mm x 100 mm



See more K-Wires on **Page 136.**

### Twist Drill



Product Code	Ø (mm)	for Screw Ø (mm)	Length (mm)	Connection
148-0080-15	1.5	for 2.0 screws	70/30	round shaft
148-0080-18	1.8	for 2.4 screws	125/25	round shaft



See more on **Page 199.**

Product Code	Ø (mm)	for Screw Ø (mm)	Length (mm)	Connection
148-0081-15	1.5	for 2.0 screws	85/60	AO QC
148-0081-18	1.8	for 2.4 screws	125/25	AO QC

### Screwdriver Shaft LeiStar

AO connection, self-holding  
(no Holding Sleeve needed)



Product Code	Description
128-1520-20	T8, for 2.0 / 2.4 mm screws, 60 mm in length
128-2024-08	T8 for 2.0 / 2.4 mm screws, 100 mm in length

### Screwdriver Shaft Hexagonal

AO connection (Holding Sleeve recommended)



Product Code	Description
128-0900-15	for 2.0 mm Screws, 100 mm long
128-0900-20	for 2.4 mm Screws, 100 mm long

More Screwdriver Shafts on **Page 200.**

### Holding Sleeve

for Hexagonal Screwdriver Shafts

Product Code	Size
128-0940-24	2.0 / 2.4 mm



### Screwdriver Handle

Silicone, AO-Connection  
sterilizable up to 134°C / 273°F



247-0103-00

MADE IN  
GERMANY



## TTA Standard

### Made in Germany

TTA Standard implants are manufactured by Rita Leibinger with a high quality.

### Titanium Implants Available In Many Sizes

Our TTA Standard implants are available from very small to very large sizes. All implants are made of Titanium.



### Cutable Cages

Besides standard cages we offer cuttable cages, too. This allows you to adjust the depth of each cage yourself.



### Affordable


Because you are buying directly from the manufacturer, we can offer all implants at affordable pricing.



### Convenience + Great Customer Service

In addition to our Standard TTA Implants, we also offer TTA RAPID, and many other implant systems. And because we manufacture the implants ourselves, we can assist you directly with your needs.



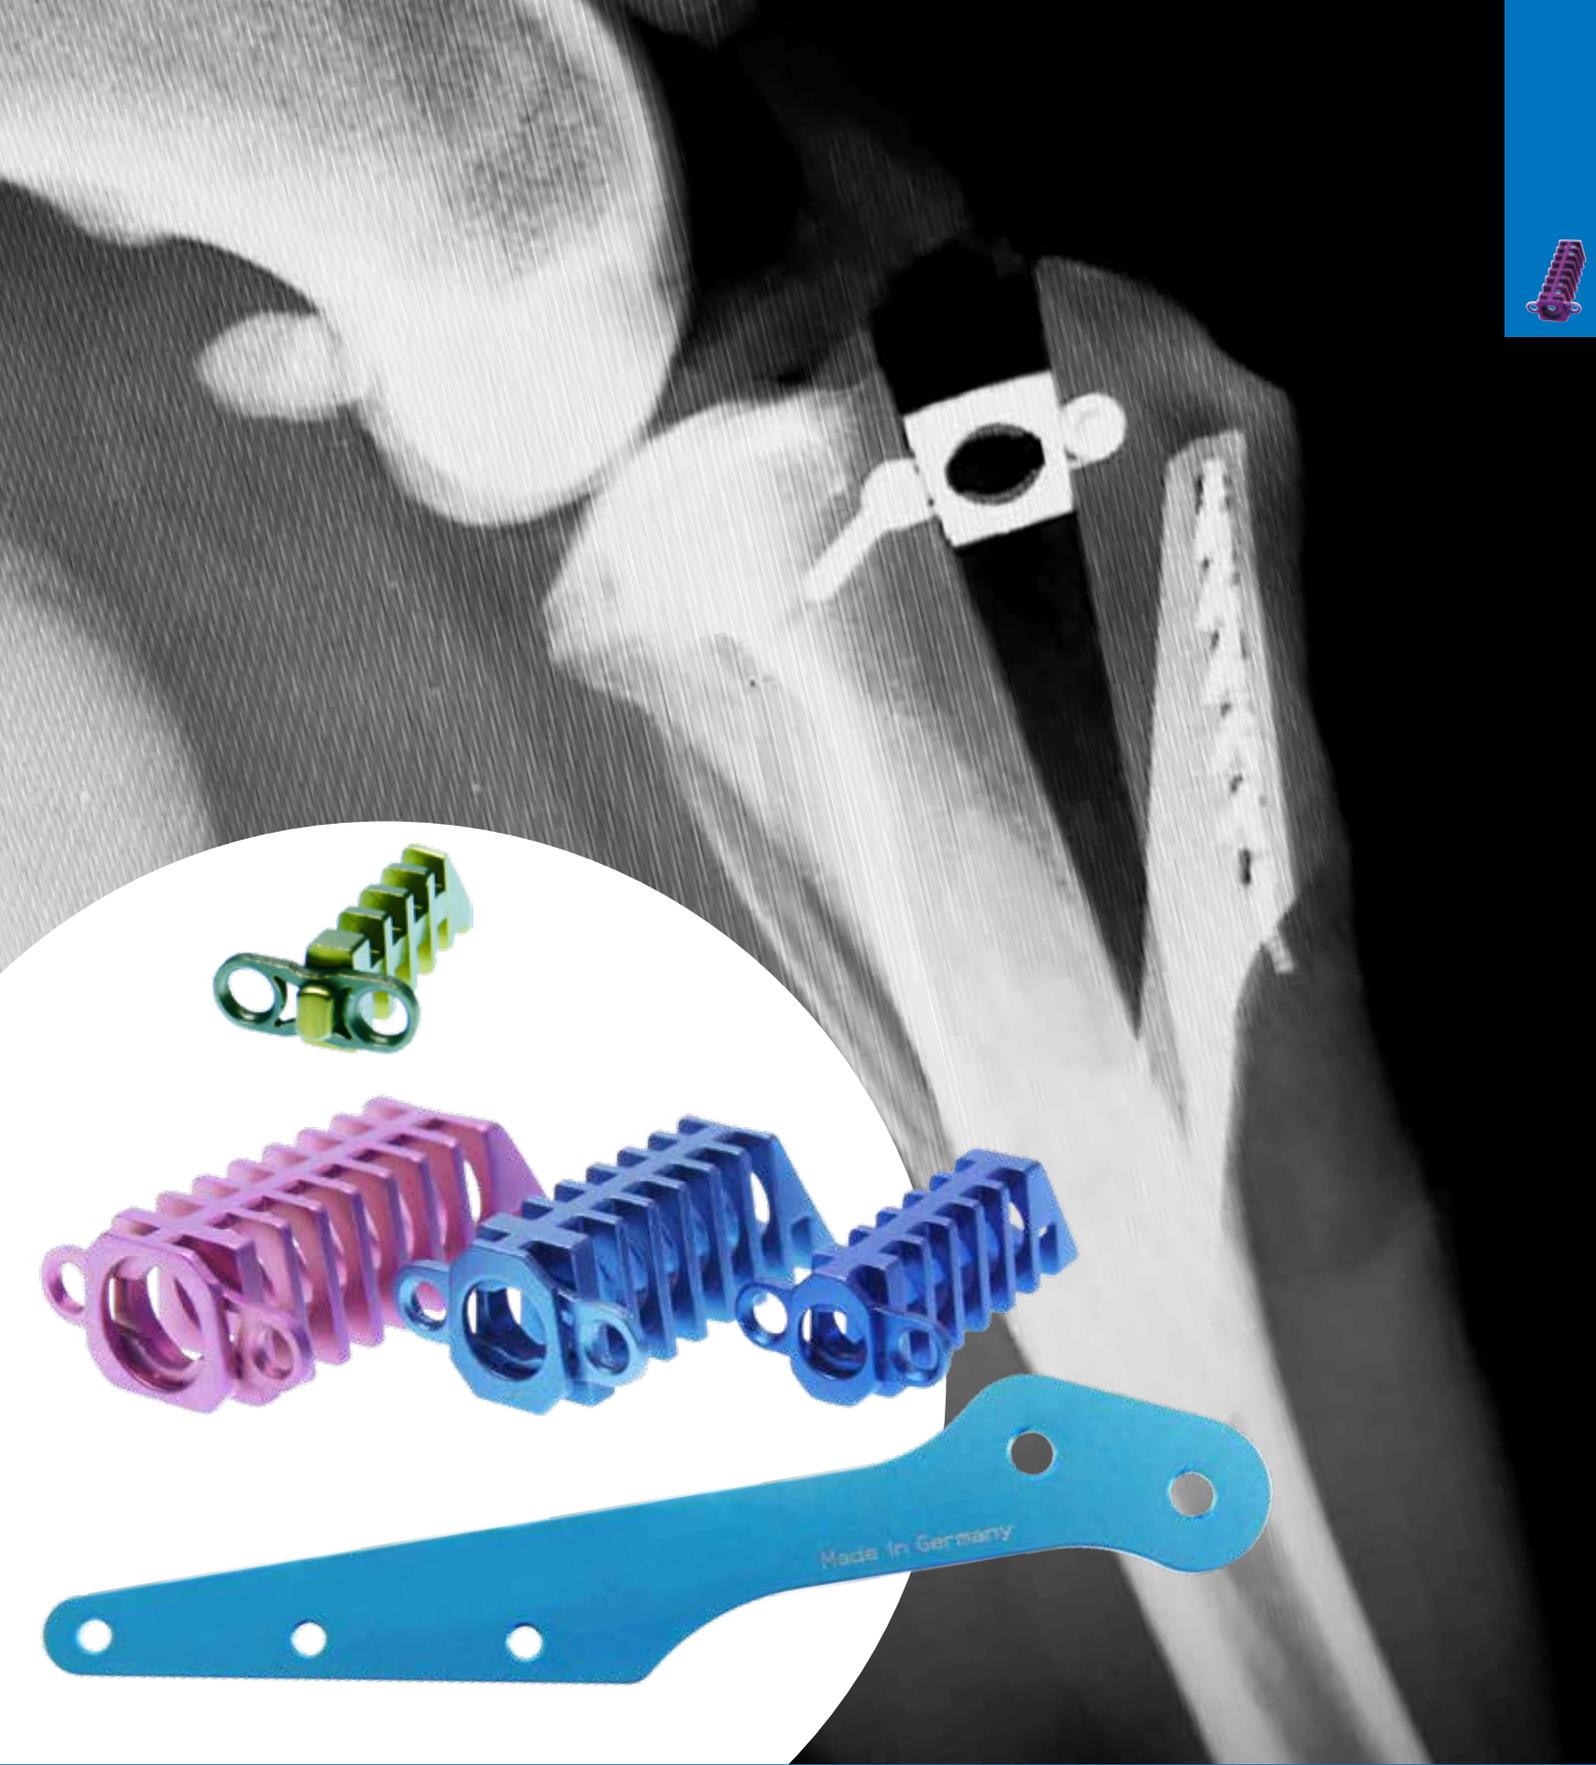

# TTA STANDARD

**R** RITA  
LEIBINGER  
MEDICAL

### TTA Implant Standard Set


Contains:

- 1 TTA Implant Tray with Lid
- 1 of each TTA Cage 3mm - 15mm (24 total)
- 2 of each 2.4mm Screw (6-40mm, 36 total)
- 2 of each 2.7mm Screw (6-40mm, 36 total)
- 2 of each 3.5mm Screw (10-50mm, 36 total)
- 1 of each Fork Standard Style 3-8
- 1 of each Plate Standard Style 3-8

**230-2020-00**

Tray without contents

**230-2080-00**

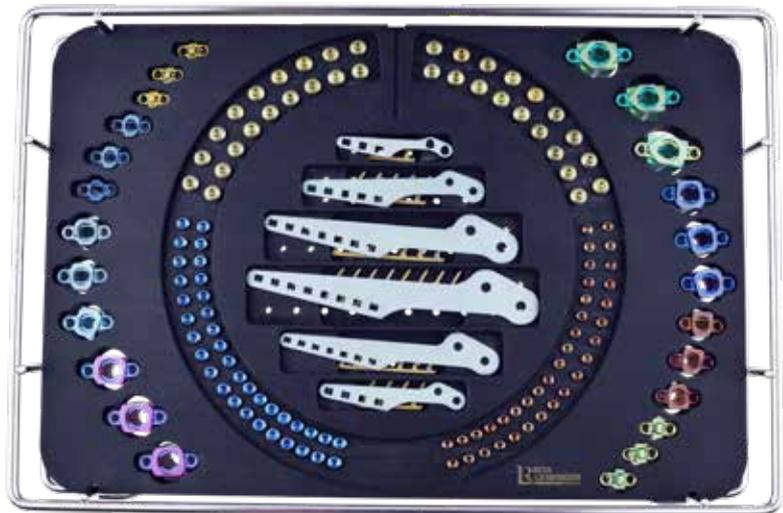

### TTA Implant ESY Set


Contains:

- 1 TTA Implant Tray with Lid
- 1 of each TTA Cage 3mm - 15mm (24 total)
- 2 of each 2.4mm Screw (6-40mm, 36 total)
- 2 of each 2.7mm Screw (6-40mm, 36 total)
- 2 of each 3.5mm Screw (10-50mm, 36 total)
- 1 of each ESY Plate Style 3-8

**230-2040-00**

Tray without contents

**230-2080-00**

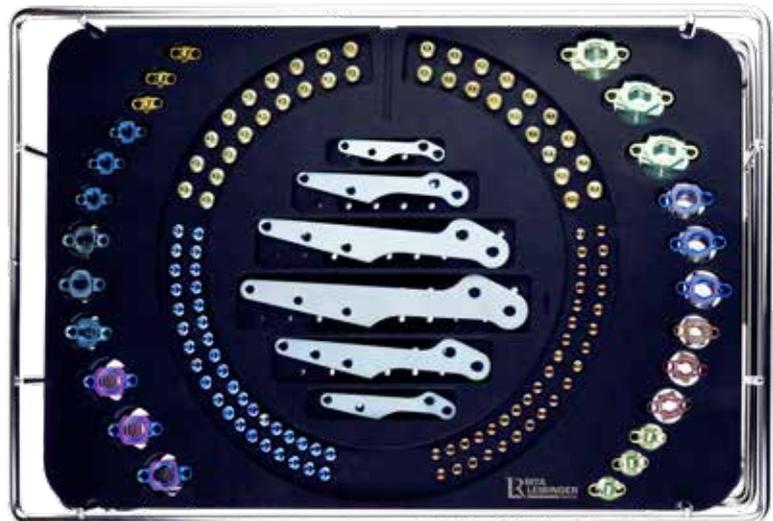

### Sterilization Container

See Sterilization Containers for Implants and Instruments Trays on **Page 204**.



## TTA Cages

## TTA Cuttable Cages

## TTA Standard Plates

### Cages

Titanium



Product Code	Size (w/d)
230-2162-310	3/10
230-2162-313	3/13
230-2162-316	3/16
230-2162-319	3/19
230-2162-4512	4.5/12
230-2162-4515	4.5/15
230-2162-4518	4.5/18
230-2162-616	6/16
230-2162-619	6/19

Product Code	Size (w/d)
230-2162-622	6/22
230-2162-7513	7.5/13
230-2162-7516	7.5/16
230-2162-7519	7.5/19
230-2162-7522	7.5/22
230-2162-919	9/19
230-2162-922	9/22
230-2162-925	9/25

Product Code	Size (w/d)
230-2162-10519	10.5/19
230-2162-10522	10.5/22
230-2162-10525	10.5/25
230-2162-1222	12/22
230-2162-1225	12/25
230-2162-1228	12/28
230-2162-1525	15/25
230-2162-1528	15/28
230-2162-1531	15/31

### Cutttable Cages

Titanium

Product Code	Size (w/d)
230-2163-622	6/22
230-2163-7524	7.5/24
230-2163-926	9/26


Product Code	Size (w/d)
230-2163-10528	10.5/28
230-2163-1230	12/30
230-2163-1532	15/32



### Forks

Titanium

Product Code	Prongs
230-2161-03	3
230-2161-04	4



Product Code	Prongs
230-2161-05	5
230-2161-06	6

Product Code	Prongs
230-2161-07	7
230-2161-08	8

### Plates Standard

Titanium

Product Code	Holes
230-2160-03	3
230-2160-04	4



Product Code	Holes
230-2160-05	5
230-2160-06	6

Product Code	Holes
230-2160-07	7
230-2160-08	8

### ESY TTA Plate

Titanium



Product Code	Specification	
	Holes	Style
230-155-03	2	3
230-155-04	2	4

Product Code	Specification	
	Holes	Style
230-155-05	2	5
230-155-06	3	6

Product Code	Specification	
	Holes	Style
230-155-07	3	7
230-155-08	3	8

TTA Spacers Titanium


For Patella Luxation



Product Code	Size (mm)
246-008-02	2
246-008-04	4
246-008-06	6

2.4 Self Tapping Screws Titanium

Hexagonal or LeiStar head, self tapping with three flute cutting edge



Length (mm)	Hexagonal	LeiStar
6	245-224-06	245-524-06
8	245-224-08	245-524-08
10	245-224-10	245-524-10
12	245-224-12	245-524-12
14	245-224-14	245-524-14
16	245-224-16	245-524-16
18	245-224-18	245-524-18
20	245-224-20	245-524-20
22	245-224-22	245-524-22
24	245-224-24	245-524-24
26	245-224-26	245-524-26
28	245-224-28	245-524-28
30	245-224-30	245-524-30
32	245-224-32	245-524-32
34	245-224-34	245-524-34
36	245-224-36	245-524-36
38	245-224-38	245-524-38
40	245-224-40	245-524-40

See more screw lengths on **Page 126.**

Screw Racks on **Page 198.**






## TTA Screws 2.7

## TTA Screws 3.5

### 2.7 Self Tapping Screws Titanium


Hexagonal or LeiStar head, self tapping with three flute cutting edge



Length (mm)	Hexagonal	LeiStar
6	245-227-06	245-527-06
8	245-227-08	245-527-08
10	245-227-10	245-527-10
12	245-227-12	245-527-12
14	245-227-14	245-527-14
16	245-227-16	245-527-16
18	245-227-18	245-527-18
20	245-227-20	245-527-20
22	245-227-22	245-527-22
24	245-227-24	245-527-24
26	245-227-26	245-527-26
28	245-227-28	245-527-28
30	245-227-30	245-527-30
32	245-227-32	245-527-32
34	245-227-34	245-527-34
36	245-227-36	245-527-36
38	245-227-38	245-527-38
40	245-227-40	245-527-40

### 3.5 Self Tapping Screws Titanium

Hexagonal or LeiStar head, self tapping with three flute cutting edge



Length (mm)	Hex Head	LeiStar
8	245-235-08	
10	245-235-10	
12	245-235-12	245-535-12
14	245-235-14	245-535-14
16	245-235-16	245-535-16
18	245-235-18	245-535-18
20	245-235-20	245-535-20
22	245-235-22	245-535-22
24	245-235-24	245-535-24
26	245-235-26	245-535-26
28	245-235-28	245-535-28
30	245-235-30	245-535-30
32	245-235-32	245-535-32
34	245-235-34	245-535-34
36	245-235-36	245-535-36
38	245-235-38	245-535-38
40	245-235-40	245-535-40
45	245-235-45	245-535-45
50	245-235-50	245-535-50
55	245-235-55	245-535-55
60	245-235-60	245-535-60

Drill Guides for Forks

Product Code	Holes
246-001-04	4
246-001-08	8



Fork Inserter

246-002-00



Pin

Size 1.9 mm

246-006-19



Drill Sleeves

Product Code	Size (mm)
164-0070-18	1.5/1.8
164-0070-27	2.0/2.7
164-0070-35	2.5/3.5



Drill Bits



Product Code	Ø (mm)	Length (mm)	Connection
148-0080-18	1.8	125/25	straight shank
148-0080-20	2.0	85/70	straight shank
148-0080-25	2.5	95/80	straight shank

Product Code	Ø (mm)	Length (mm)	Connection
148-0081-18	1.8	125/25	AO Schaft
148-0081-20	2.0	100/75	AO Schaft
148-0081-25	2.5	110/85	AO Schaft

Depth Gauge

For 2.4 | 2.7 | 3.5 screws  
maximal measurement 60 mm

164-2735-60



Screwdriver Handle

Silicone, AO-Connection  
sterilizable up to 134°C / 273°F

247-0103-00





Screwdriver

TTA RAPID Spreader

Bone Holding Forceps

Screwdriver LeiStar

AO connection, self-holding (no Holding Sleeve needed)

Product Code	Description
128-1520-20	T8, for 2.0 and 2.4 mm Screws
128-2735-10	T10, for 2.7 and 3.5 mm Screws



Screwdriver Hex Insert

AO connection, self-holding, (Holding Sleeve recommended)

Product Code	Description
128-0900-20	for 2.4 mm Screws
128-0900-25	for 2.7 and 3.5 mm Screws



Holding Sleeve

for Hexagonal Screwdriver Shafts

Product Code	Size
128-0940-24	2.0 / 2.4 mm
128-0940-25	2.7 / 3.5 mm



Plate Holding Forceps

16 cm angled

164-0050-16



TTA RAPID® Spreader

With tensioning and fixation screw, 16 cm

132-4080-16



Boneholding Forceps

21.5 cm, with spin lock

128-0525-21



TTA Bending Iron

120 mm

132-4020-00



# LeiLOX TPLO



## Tradition improved and Made Affordable

LeiLOX TPLO implants are made in Germany by Rita Leibinger. Because you are buying directly from the manufacturer, we can offer them at an affordable price.



## Multiaxial Locking

The screws can be locked in a 90° angle with a 12° deviation in any direction. This allows you to angle the screws away from vital structures. The robust LeiStar screw head can be locked firmly into the plate.



## Anatomically Shaped Limited Contact Dynamic Compression Plates

The LeiLOX TPLO plates are contoured to match the anatomic shape of the bone. This makes it easier to place the plate in an optimal position.

The plate features limited contact dynamic compression to minimize vascular damage to the plated bone segment.



## Double Compression

Two precisely designed compression holes enable a very tight compression of the osteotomy.



## Interchangeable 2.7 & 3.5mm and 2.0 & 2.4mm Screws

Because the screwheads are identical, all Stainless Steel 2.7/3.5 LeiLOX plates (TPLO and fracture systems) work with 2.7mm as well as 3.5mm screws in all of the plate sizes. Same applies for the 2.0/2.4 systems. This offers flexibility and ideal implant selection for each patient. Moreover, this saves on inventory cost.

High Performance TPLO Sawblades are available. The Titanium Nitrate coating allows them to last significantly longer than standard blades.

# LeiLOX

**TPLO** Locking System



Special Thanks to  
Dr. Ulrich Rytz

## LeiLOX TPLO

**R** RITA  
LEIBINGER  
MEDICAL

## LEILOX TPLO TECHNIQUE

### Pre-Operative Planning

#### Positioning the Patient for Radiographs

Proper positioning is essential for accurate planning. By ensuring proper positioning of the limb, accurate radiographs with consistent appearance of anatomic landmarks can be obtained for TPLO pre-operative planning, allowing for precise measurements.

To obtain lateral radiographic views of the stifle joint and tibia, the patient is positioned in lateral recumbency on a radiographic table, with the stifle and tarsus positioned at 90°. The patient is best sedated to ensure optimal positioning. Orthogonal radiographs are taken with the beam centered over the stifle joint.

It is important to know that any internal or external rotation of the tibia can affect how the tibial plateau appears on the X-ray. This rotation can occur due to incorrect positioning of the affected limb or failure to center the X-ray beam accurately over the stifle joint.

#### Determining the Tibial Plateau Angle (TPA)



**Draw the functional axis (FA)**, also known as the weight bearing axis or mechanical tibial axis. Draw a line from the intercondylar eminence or tibial eminence proximally to the center of the tarsal joint or talocrural joint distally.


**Draw the tibial plateau line (TP)**. To check correctness of the tibial plateau line, the cranial and caudal points of this line should be equally distant from the intercondylar eminence.

Draw a line perpendicular to the FA, where it intersects with the TP. The **TPA** is the angle between this line and TP.

#### Determining Saw Blade Radius

Considering the patient's weight and bone size, a suitable curved saw blade is chosen, ranging from 9mm to 33mm in radius. The saw blade radius is determined as follows:

- The osteotomy is centered at the intercondylar eminence (**X**)
- A line is drawn from the tibial crest to the caudal edge of the medial tibial plateau (**Line A**). Mark the cranial third of this line (Point **B**) and measure the distance between points B and X. Choose the saw blade radius (**R**) closest to this distance.
- With the center at X, draw a circle with a radius equivalent to the selected saw blade radius (R).
- Note down the following measurements:
  - **D1** - Draw a line perpendicular to the cranial border of the tibia (**Line C**) starting from the insertion of the patellar tendon to the osteotomy line, and measure this distance. In large dogs, this distance should be at least 1 cm.
  - **D2** - From the cranial end of D1 to the cranial point of the osteotomy
  - **D3** - From the caudal point of the osteotomy to the caudal end of the tibia
- Also check to make sure that the osteotomy line is perpendicular to the caudal border of the tibia.

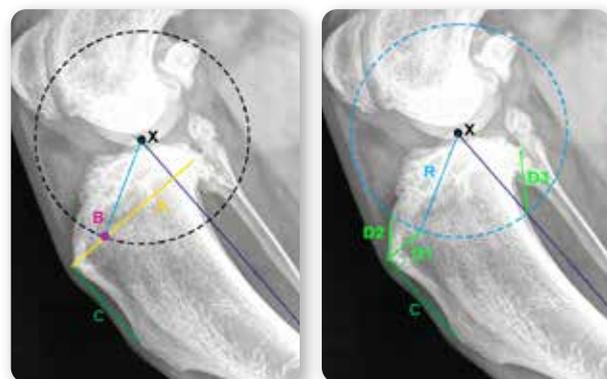

With the pre-op TPA and the selected saw blade radius (R) values at hand, determine the amount of rotation with the help of the TPLO Rotation Chart. The goal is to achieve a post-op TPA of 4-6 degrees, effectively neutralizing abnormal shear forces resulting from cruciate ligament deficiency and restoring biomechanical stability.

Original Author (English version):

**Dr. Yves Samoy, DVM, PhD, Dipl. ECVSMR,**  
Certified Small Animal Rehabilitation Practitioner (UGent)

See TPLO Rotation Chart on **Page 46**.

View online or download the rotation chart here →



[tplo.leibinger.vet](http://tplo.leibinger.vet)

LEARN FROM THE BEST

**WORKSHOPS**

Learn the TPLO Technique in one of our workshops.

[academy.leibinger.vet](http://academy.leibinger.vet)



# LEILOX TPLO TECHNIQUE

## Surgery Protocol

### Positioning of the Patient

The dog is placed in a dorsal recumbency with the affected limb suspended from a stand. Make sure that the dog's paws are not fixed too tightly, since the affected limb will be put against the table later in the surgery. TPLO is performed through a medial skin incision.




#### Use of a Jig

The use of a jig is advised when performing a leveling osteotomy.

### Placement of the Jig

- 1 The joint surface is marked with a needle. About 3 to 4 mm below is the insertion point of the proximal pin for the TPLO Jig.
- 2 The proximal pin is inserted in a 90° angle to the joint surface.

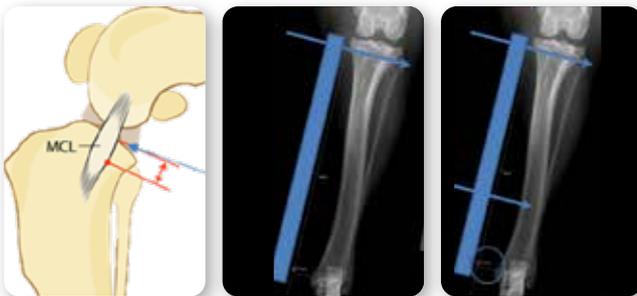


- 3 The distal pin is placed. Take care to not tilt the jig. The pins must be parallel to each other, and absolutely perpendicular to the jig.

### Making the Osteotomy

The location of the osteotomy is determined with the use of the D1-D3 measurements taken during pre-op planning.

- 1 Using a radial oscillating saw, perform a partial osteotomy, making sure that the cut is parallel to the pins and perpendicular to the jig.
- 2 The cut is made approximately half-way (1/2) or a third (1/3) of the way through the bone. Then, measure and make the following markings for the rotation as determined during pre-op planning:
  - Position the first mark on the proximal bone fragment adjacent to the edge of the osteotomy, ensuring it is situated cranially to the midpoint of the osteotomy.
  - A second mark is then made on the distal bone fragment at the designated distance from the first mark, as determined by the TPLO Rotation Chart during pre-operative planning.

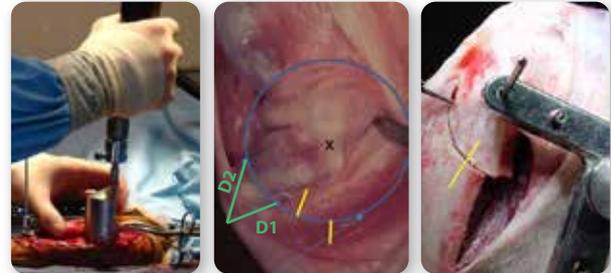


- 3 Complete the cut, loosen the jig, and rotate the proximal bone fragment to align the two markings. Once the correct rotation has been achieved, stabilize the osteotomy by placing a K-Wire across the tibial tuberosity.

### Placement of the TPLO Plate

Place the TPLO Plate, securing it in place with K-Wires. At this point, the jig may be loosened or completely removed.

The screws are inserted in the following (recommended) sequence:

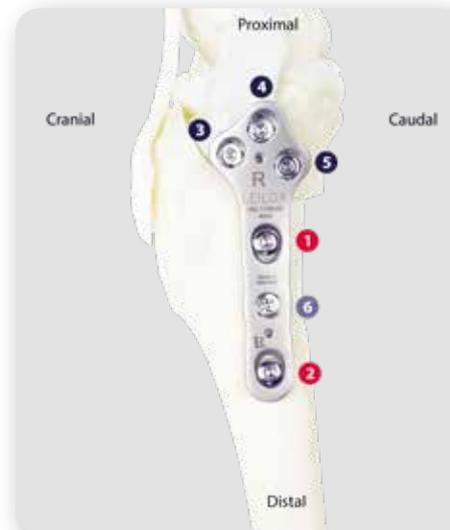

**1 2**

Insert standard **cortical screws** 1 and then 2 into the compression holes. Do not tighten yet.

**3 4 5**

Insert **locking screws** 3, 4, and then 5 into the plate head and tighten.

**1 2**

Remove K-Wires (IMPORTANT!) and tighten screws 1 and 2 for a strong compression.

**6**

Insert **locking screw** 6 and tighten.

# LeiLOX TPLO Rotation Chart

		Pre-operative Tibia Plateau Angle (TPA)												
		15°	16°	17°	18°	19°	20°	21°	22°	23°	24°	25°	26°	27°
		Rotation (mm) - Provides Resultant 5° TPA												
Saw Blade Size / Radius	9 mm	1.6	1.7	1.9	2.0	2.2	2.4	2.5	2.7	2.8	3.0	3.1	3.3	3.5
	12 mm	2.1	2.3	2.5	2.7	2.9	3.1	3.4	3.6	3.8	4.0	4.2	4.4	4.6
	15 mm	2.6	2.9	3.1	3.4	3.7	3.9	4.2	4.5	4.7	5.0	5.2	5.5	5.8
	18 mm	3.1	3.5	3.8	4.1	4.4	4.7	5.0	5.3	5.7	6.0	6.3	6.6	6.9
	21 mm	3.7	4.0	4.4	4.8	5.1	5.5	5.9	6.2	6.6	7.0	7.3	7.7	8.1
	24 mm	4.2	4.6	5.0	5.4	5.9	6.3	6.7	7.1	7.5	8.0	8.4	8.8	9.2
	27 mm	4.7	5.2	5.7	6.1	6.6	7.1	7.5	8.0	8.5	9.0	9.4	9.9	10.4
	30 mm	5.2	5.8	6.3	6.8	7.3	7.9	8.4	8.9	9.4	9.9	10.5	11.0	11.5
	33 mm	5.8	6.3	6.9	7.5	8.1	8.6	9.2	9.8	10.4	10.9	11.5	12.1	12.7

		Pre-operative Tibia Plateau Angle (TPA)												
		28°	29°	30°	31°	32°	33°	34°	35°	36°	37°	38°	39°	40°
		Rotation (mm) - Provides Resultant 5° TPA												
Saw Blade Size / Radius	9 mm	3.6	3.8	3.9	4.1	4.2	4.4	4.6	4.7	4.9	5.0	5.2	5.3	5.5
	12 mm	4.8	5.0	5.2	5.4	5.7	5.9	6.1	6.3	6.5	6.7	6.9	7.1	7.3
	15 mm	6.0	6.3	6.5	6.8	7.1	7.3	7.6	7.9	8.1	8.4	8.6	8.9	9.2
	18 mm	7.2	7.5	7.9	8.2	8.5	8.8	9.1	9.4	9.7	10.1	10.4	10.7	11.0
	21 mm	8.4	8.8	9.2	9.5	9.9	10.3	10.6	11.0	11.4	11.7	12.1	12.5	12.8
	24 mm	9.6	10.1	10.5	10.9	11.3	11.7	12.1	12.6	13.0	13.4	13.8	14.2	14.7
	27 mm	10.8	11.3	11.8	12.3	12.7	13.2	13.7	14.1	14.6	15.1	15.6	16.0	16.5
	30 mm	12.0	12.6	13.1	13.6	14.1	14.7	15.2	15.7	16.2	16.8	17.3	17.8	18.3
	33 mm	13.2	13.8	14.4	15.0	15.6	16.1	16.7	17.3	17.9	18.4	19.0	19.6	20.2

### Rotation Calculation

$$X \text{ (mm)} = [2\pi \text{ (saw blade diameter)}] (\text{TPA}-5^\circ/360^\circ)$$

According to: TPLO principles, patient selection, and preoperative planning  
by Derek B. Fox, DVM, PhD, Dipl ACVS, Assistant Professor, Missouri, USA



## Patient Weight Guide for LeiLOX TPLO Plates

The weight ranges are suggestions based on the recommendations of our veterinary consultants. This table only serves as a guide. It is up to the veterinarian to assess and determine the correct implant size, material type, and configuration to use for his patient, as well as its application and the technique to be employed.

		LeiLOX TPLO Implant Size
<b>Weight Range</b>	Less than <b>10 kg</b>	2.0 mm
	<b>8 - 18 kg</b>	2.4 mm
	<b>15 - 30 kg</b>	2.7 mm
	<b>25 - 40 kg</b>	3.5 mm
	More than <b>35 kg</b>	3.5 mm broad

LEARN FROM THE BEST

### WORKSHOPS

Learn the TPLO Technique in one of our workshops.

[academy.leibinger.vet](https://academy.leibinger.vet)

## Treating CrCL Rupture + Patella Luxation with TPLO

Tibial Plateau Leveling Osteotomy (TPLO) is a widely recognized surgical technique and remains a globally popular choice for addressing cranial cruciate ligament (CrCL) tears in dogs and cats. Joint instability following a ligament injury can exacerbate an existing, mild patellar luxation. CrCL injuries in susceptible dogs, particularly those with pre-existing anatomical predispositions, might also indirectly affect the alignment and tracking of the patella, potentially leading to luxation.

Conversely, an existing patellar luxation can increase the risk of CrCL rupture due to limb alignment abnormalities and joint instability.

When both conditions are present, addressing both is crucial for ensuring optimal joint stability and function.



**NEW**

### LeiLOX TPLO Patella Spacers Treating both conditions simultaneously with TPLO

#### One-surgery solution

The **LeiLOX TPLO Patella Spacers** can be seamlessly implanted together with our LeiLOX TPLO Plates in a challenging case of a CrCL rupture and a concomitant patella luxation.

Learn this technique in one of our workshops:

[academy.leibinger.vet](https://academy.leibinger.vet)

See TPLO Patella Luxation Spacers on **Page 58**.

### 2.0 / 2.4 TPLO Set

Contains:

- 1 TPLO Implants and Instruments Tray with Lid
- 2 of each TPLO Plate
- 3 of each Cortical Screw (8-18mm // 8-22mm, 42 total)
- 5 of each Locking Screw (6-24mm // 6-30mm, 115 total)
- 2 Drills (1.5 & 1.8mm)
- 5 K-Wires
- 2x2 Locking Drill Guides
- 2 Compression Drill Guides
- 1 TPLO Jig
- 1 Screwdriver Handle
- 1 Screwdriver Shaft T8
- 1 Depth Gauge



**142-0150-00**

Tray without contents

**142-2800-10**



### Sterilization Container

See Sterilization Containers for Implants and Instruments Trays on **Page 204**.

### 2.0 / 2.4 LeiLOX TPLO Locking Plate



LeiLOX TPLO Locking Plate, 2.0 mm, left, 33 mm, Stainless Steel

**142-1120-10**



LeiLOX TPLO Locking Plate, 2.0 mm, right, 33 mm, Stainless Steel

**142-1120-00**



LeiLOX TPLO Locking Platte, 2.4 mm, left, 37 mm, Stainless Steel

**142-1124-10**



LeiLOX TPLO Locking Plate, 2.4 mm, right, 37 mm, Stainless Steel

**142-1124-00**

## TPLO Screws Locking & Non-Locking 2.0/2.4 Stainless Steel

### 2.0 / 2.4 LeiLOX Locking Screw Stainless Steel

For LeiLOX Locking Systems, LeiStar T8  
self-holding (T8 Shaft from Rita Leibinger recommended)  
self-tapping with three flute cutting edge



	2.0 mm	2.4 mm
Length (mm)	Product Code	Product Code
06	242-120-06	242-124-06
08	242-120-08	242-124-08
10	242-120-10	242-124-10
12	242-120-12	242-124-12
14	242-120-14	242-124-14
16	242-120-16	242-124-16
18	242-120-18	242-124-18
20	242-120-20	242-124-20
22	242-120-22	242-124-22
24	242-120-24	242-124-24
26		242-124-26
28		242-124-28
30		242-124-30

### 2.0 / 2.4 Cortical Screw Stainless Steel

LeiStar T8, Non-Locking  
self-holding (T8 Shaft from Rita Leibinger recommended)  
self-tapping with three flute cutting edge



	2.0 mm	2.4 mm
Length (mm)	Product Code	Product Code
08	245-620-08	245-624-08
10	245-620-10	245-624-10
12	245-620-12	245-624-12
14	245-620-14	245-624-14
16	245-620-16	245-624-16
18	245-620-18	245-624-18
20		245-624-20
22		245-624-22

See more screw lengths on **Page 126.**

Screw Racks on **Page 198.**



**2.7 / 3.5 TPLO Implant Set**

Contains:

- 1 TPLO Implant Tray with Lid
- 2 of each TPLO Plate
- 3 of each Cortical Screw (16-34mm, 60 total)
- 5 of each Locking Screw (16-46mm, 160 total)

**142-0100-02**

Tray without contents

**142-0100-10**



**2.7 / 3.5 LeiLOX TPLO Locking Plate**



LeiLOX TPLO Locking Plate, 2.7 mm, left, 46 mm, Stainless Steel

**142-1127-10**



LeiLOX TPLO Locking Plate, 2.7 mm, right, 46 mm, Stainless Steel

**142-1127-00**



LeiLOX TPLO Locking Plate, 3.5 mm, left, 66 mm, Stainless Steel

**142-1135-10**



LeiLOX TPLO Locking Plate, 3.5 mm, right, 66 mm, Stainless Steel

**142-1135-00**



LeiLOX TPLO Locking Plate, broad, 3.5 mm, left, 75 mm, Stainless Steel

**142-1135-60**



LeiLOX TPLO Locking Plate, broad, 3.5 mm, right, 75 mm, Stainless Steel

**142-1135-50**

## TPLO Screws Locking & Non-Locking 2.7/3.5 Stainless Steel

### 2.7 / 3.5 LeiLOX Locking Screw Stainless Steel

For LeiLOX Locking Systems, LeiStar T10 self-holding (T10 Shaft from Rita Leibinger recommended) self-tapping with three flute cutting edge



	2.7 mm	3.5 mm
Length (mm)	Product Code	Product Code
10	242-127-10	242-135-10
12	242-127-12	242-135-12
14	242-127-14	242-135-14
16	242-127-16	242-135-16
18	242-127-18	242-135-18
20	242-127-20	242-135-20
22	242-127-22	242-135-22
24	242-127-24	242-135-24
26	242-127-26	242-135-26
28	242-127-28	242-135-28
30	242-127-30	242-135-30
32	242-127-32	242-135-32
34	242-127-34	242-135-34
36	242-127-36	242-135-36
38	242-127-38	242-135-38
40	242-127-40	242-135-40
42	242-127-42	242-135-42
44	242-127-44	242-135-44
46	242-127-46	242-135-46
48	242-127-48	242-135-48
50	242-127-50	242-135-50
52		242-135-52
54		242-135-54
56		242-135-56
58		242-135-58
60		242-135-60
62		242-135-62
64		242-135-64
66		242-135-66
68		242-135-68
70		242-135-70

### 2.7 / 3.5 Cortical Screw Stainless Steel

LeiStar T10, Non-Locking self-holding (T10 Shaft from Rita Leibinger recommended) self-tapping with three flute cutting edge



	2.7 mm	3.5 mm
Length (mm)	Product Code	Product Code
16	245-627-16	245-635-16
18	245-627-18	245-635-18
20	245-627-20	245-635-20
22	245-627-22	245-635-22
24	245-627-24	245-635-24
26	245-627-26	245-635-26
28	245-627-28	245-635-28
30	245-627-30	245-635-30
32	245-627-32	245-635-32
34	245-627-34	245-635-34

See more screw lengths on [Page 126](#).



#### TPLO Saw Blades

See radial saw blades for TPLO and CBLO in various radii on [Page 191](#).




#### Screw Racks

See screw racks for 1.5mm up to 3.5mm screws on [Page 198](#).



#### TPLO Instruments

See essential instruments for a TPLO Surgery on [Page 78](#).



#### Instrument Set

See Instrument Set for TPLO / CBLO / CCWO on [Page 78](#).

# LeiLOX TPLO Swing



## Titanium for Best Biocompatibility

LeiLOX TPLO Swing implants are made of medical grade Titanium, which makes them very durable but lightweight, highly biocompatible, and low in temperature sensitiveness.



## Multiaxial Locking

The screws can be locked in a 90° angle with a 12° deviation in any direction. This allows you to angle the screws away from vital structures. The robust LeiStar screw head can be locked firmly into the plate.



## Anatomically Shaped Limited Contact Dynamic Compression Plates

The LeiLOX TPLO Swing plates are contoured to match the anatomic shape of the bone. This makes it easier to place the plate in an optimal position.

The plate features limited contact dynamic compression to minimize vascular damage to the plated bone segment.



## Double Compression

Two precisely designed compression holes enable a very tight compression of the osteotomy.



## Interchangeable 2.7 & 3.5mm and 2.0 & 2.4mm Screws

Because the screwheads are identical, all Titanium 2.7/3.5 LeiLOX plates (TPLO Swing, CBLO, and CCWO systems) work with 2.7mm as well as 3.5mm screws in all of the plate sizes. Same applies for the 2.0/2.4 systems. This offers flexibility and ideal implant selection for each patient. Moreover, this saves on inventory cost.

High Performance Sawblades are available. The Titanium Nitrate coating allows them to last significantly longer than standard blades.

# LeiLOX

## TPLO Swing

TPLO Swing  
Titanium



Special Thanks to  
Dr. Matan Or

# LeiLOX TPLO SWING

**R** RITA  
LEIBINGER  
MEDICAL

**2.0 / 2.4 TPLO Swing Set**

Contains:

- 1 TPLO Implants and Instruments Tray with Lid
- 2 of each TPLO Swing Locking Plate
- 3 of each Cortical Screw
- (2.0, 8-18mm // 2.4, 8-22mm, 42 total)
- 5 of each Locking Screw
- (2.0, 6-24mm // 2.4, 6-30mm, 115 total)
- 2 Drills (1.5 & 1.8mm)
- 5 K-Wires
- 2x2 Locking Drill Guides
- 2 Compression Drill Guides
- 1 TPLO Jig
- 1 Screwdriver Handle
- 1 Screwdriver Shaft T8
- 1 Depth Gauge



**142-2820-24**

Tray without contents

**142-2800-10**



**Sterilization Container**

See Sterilization Containers for Implants and Instruments Trays on **Page 204**.

**2.0 / 2.4 LeiLOX TPLO Swing Locking Plates Titanium**



LeiLOX TPLO Swing Locking Plate  
2.0 mm, left, 33 mm, Titanium

**142-2820-10**



LeiLOX TPLO Swing Locking Plate  
2.0 mm, right, 33 mm, Titanium

**142-2820-00**



LeiLOX TPLO Swing Locking Plate  
2.4 mm, left, 37 mm, Titanium

**142-2824-10**



LeiLOX TPLO Swing Locking Plate  
2.4 mm, right, 37 mm, Titanium

**142-2824-00**

## TPLO Screws Locking & Non-Locking 2.0/2.4 Titanium

### 2.0 / 2.4 LeiLOX Locking Screw Titanium

For LeiLOX Locking Systems, LeiStar T8  
self-holding (T8 Shaft from Rita Leibinger recommended)  
self-tapping with three flute cutting edge



	2.0 mm	2.4 mm
Length (mm)	Product Code	Product Code
06	242-220-06	242-224-06
08	242-220-08	242-224-08
10	242-220-10	242-224-10
12	242-220-12	242-224-12
14	242-220-14	242-224-14
16	242-220-16	242-224-16
18	242-220-18	242-224-18
20	242-220-20	242-224-20
22	242-220-22	242-224-22
24	242-220-24	242-224-24
26	242-220-26	242-224-26
28	242-220-28	242-224-28
30	242-220-30	242-224-30
32		242-224-32
34		242-224-34
36		242-224-36
38		242-224-38
40		242-224-40

### 2.0 / 2.4 Cortical Screw (Non-Locking) Titanium

LeiStar T8, Non-Locking  
self-holding (T8 Shaft from Rita Leibinger recommended)  
self-tapping with three flute cutting edge



	2.0 mm	2.4 mm
Length (mm)	Product Code	Product Code
08	245-520-08	245-524-08
10	245-520-10	245-524-10
12	245-520-12	245-524-12
14	245-520-14	245-524-14
16	245-520-16	245-524-16
18	245-520-18	245-524-18
20		245-524-20
22		245-524-22

See more screw lengths on **Page 126.**

Screw Racks on **Page 198.**

**2.7 / 3.5 TPLO Swing Set**

Contains:

- 1 TPLO Implant Tray with Lid
- 2 of each TPLO Swing Plate
- 3 of each Cortical Screw (16-34mm, 60 total)
- 5 of each Locking Screw (16-46mm, 160 total)

**142-2827-35**

Tray without contents

**142-2800-20**



**2.7 / 3.5 LeiLOX TPLO Swing Locking Plates Titanium**



LeiLOX TPLO Swing Locking Plate  
2.7 mm, left, 44 mm, Titanium

**142-2827-10**



LeiLOX TPLO Swing Locking Plate  
2.7 mm, right, 44 mm, Titanium

**142-2827-00**



LeiLOX TPLO Swing Locking Plate  
3.5 mm, left, 63 mm, Titanium

**142-2835-10**



LeiLOX TPLO Swing Locking Plate  
3.5 mm, right, 63 mm, Titanium

**142-2835-00**



LeiLOX TPLO Swing Locking Plate  
3.5 mm, left, 74 mm, Titanium

**142-2835-60**



LeiLOX TPLO Swing Locking Plate  
3.5 mm, right, 74 mm, Titanium

**142-2835-50**



## TPLO Screws Locking & Non-Locking 2.7/3.5 Titanium

### 2.7 / 3.5 LeiLOX Locking Screw Titanium

For LeiLOX Locking Systems, LeiStar T10 self-holding (T10 Shaft from Rita Leibinger recommended) self-tapping with three flute cutting edge



	2.7 mm	3.5 mm
Length (mm)	Product Code	Product Code
10	242-227-10	242-235-10
12	242-227-12	242-235-12
14	242-227-14	242-235-14
16	242-227-16	242-235-16
18	242-227-18	242-235-18
20	242-227-20	242-235-20
22	242-227-22	242-235-22
24	242-227-24	242-235-24
26	242-227-26	242-235-26
28	242-227-28	242-235-28
30	242-227-30	242-235-30
32	242-227-32	242-235-32
34	242-227-34	242-235-34
36	242-227-36	242-235-36
38	242-227-38	242-235-38
40	242-227-40	242-235-40
42	242-227-42	242-235-42
44	242-227-44	242-235-44
46	242-227-46	242-235-46
48	242-227-48	242-235-48
50	242-227-50	242-235-50
52		242-235-52
54		242-235-54
56		242-235-56
58		242-235-58
60		242-235-60

See more screw lengths on **Page 126**.

### 2.7 / 3.5 Cortical Screw Titanium

LeiStar T10, Non-Locking self-holding (T10 Shaft from Rita Leibinger recommended) self-tapping with three flute cutting edge



	2.7 mm	3.5 mm
Length (mm)	Product Code	Product Code
16	245-527-16	245-535-16
18	245-527-18	245-535-18
20	245-527-20	245-535-20
22	245-527-22	245-535-22
24	245-527-24	245-535-24
26	245-527-26	245-535-26
28	245-527-28	245-535-28
30	245-527-30	245-535-30
32	245-527-32	245-535-32
34	245-527-34	245-535-34



#### TPLO Saw Blades

See radial saw blades for TPLO and CBLO in various radii on **Page 191**.



#### Screw Racks

See screw racks for 1.5mm up to 3.5mm screws on **Page 198**.



#### TPLO Instruments

See essential instruments for a TPLO Surgery on **Page 78**.



#### Instrument Set

See Instrument Set for TPLO / CBLO / CCWO on **Page 78**.

**TPLO Patella Luxation Spacers**

For LeiLOX TPLO Stainless Steel and TPLO Swing Titanium Systems

Description	Compatibility	Product Code
2.0 TPLO Patella Luxation Spacer Titanium, 2.0mm thick for 2.0 mm TPLO Locking Plates, left & right		142-8020-00
2.4 TPLO Patella Luxation Spacer Titanium, 2.0mm thick for 2.4 mm TPLO Locking Plates, left & right		142-8024-00
2.7 TPLO Patella Luxation Spacer Titanium, 2.0mm thick for 2.7 mm TPLO Locking Plates, left & right		142-8027-00
3.5 TPLO Patella Luxation Spacer Titanium, 2.0mm thick for 3.5 mm TPLO Locking Plates, left & right		142-8035-00
3.5 broad TPLO Patella Luxation Spacer Titanium, 2.0mm thick for 3.5 mm broad TPLO Locking Plates, left & right		142-8035-10

**Tibia Tappet**

For inserting TPLO Patella Luxation Spacers

Product Code	Description
142-2890-00	For 2.0 / 2.4 mm plates
142-2891-00	For 2.7/3.5 mm plates



# LEILOX TPLO PATELLA LUXATION SYSTEM

## Correction of a Patella Luxation during a TPLO Surgery

Treating concurrent cranial cruciate ligament (CrCL) rupture and patella luxation in dogs has traditionally posed a significant challenge for veterinary surgeons. However, the introduction of LeiLOX TPLO Patella Luxation Spacers has revolutionized this process, making it simpler and more efficient. By seamlessly integrating the spacer insertion into the standard Tibial Plateau Leveling Osteotomy (TPLO) procedure, surgeons can now address both conditions simultaneously with greater ease and precision.



Learn this technique in one of our workshops:  
**academy.leibinger.vet**



## TPLO + PATELLA LUXATION

The LeiLOX TPLO Patella Luxation Spacer is designed to be inserted directly beneath the TPLO plate after the rotation of the proximal bone fragment and before tightening the distal screws. This straightforward addition eliminates the need for a separate surgical approach for patella luxation correction, significantly streamlining the procedure. The specially designed tappet allows for precise lateral transposition of the tibial crest, ensuring optimal alignment and guidance of the patella.

### Osteotomy and TPLO Plate Placement

Perform a tibial plateau leveling osteotomy (TPLO) using the preselected radial saw blade, centering it in the region of the tibial eminences to achieve the desired TPA correction. Rotate the proximal tibial fragment to achieve a postoperative TPA of 4-6 degrees. Secure the LeiLOX TPLO Plate onto the proximal bone fragment with pins.

### Patella Luxation Correction Using LeiLOX TPLO Patella Luxation Spacers


#### Insertion of the First Five Screws

Insert standard cortical screws 1 and then 2 into the compression holes. Do not tighten yet. Insert locking screws 3, 4, and then 5 into the plate head and tighten.



#### Use of the Tappet:

Insert the special tappet into locking hole 6 of the LeiLOX TPLO Plate. Rotate the tappet to fixate it in the screw hole of the TPLO Plate. Rotate the pin to transpose the tibia to the lateral side until the luxation is corrected.



Flex and extend the stifle to check the alignment of the patella. Adjust the transposition with the tappet if needed to achieve optimal patellar alignment.

#### Insertion of the Patella Luxation Spacer:

Once the desired position is achieved, insert the TPLO Patella Luxation Spacers between the plate and the bone. Spacers are stackable. Remove the tappet.

#### Final Fixation

Remove any remaining pins, then tighten compression screws 1 and 2. Insert locking screw 6 and tighten. Ensure stable fixation and verify the correction of the tibial plateau angle and patella alignment through intraoperative radiography if available.

#### Closure

Close the periosteum and soft tissue layers carefully to protect the implant site, ensuring all incisions, including the distal jig pin incision, are properly closed.

# LeiLOX CBLO



## Combines the advantages of TPLO and TTA

CBLO (CORA based leveling osteotomy) is a modern osteotomy technique to level the tibia plateau, similar to TPLO. However, CBLO addresses further challenges such as secondary (late) meniscal damage, overload of the caudal cruciate ligament, reduction of proximal anatomic axis shift and the secondary translation as well as misalignment of the joint.



## Multiaxial Locking & Titanium

The screws can be locked in 90° angle with a 12° deviation in any direction. This allows you to angle the screws away from vital structures. The robust LeiStar screw head can be locked firmly into the plate.

All LeiLOX CBLO Implants are made of Titanium by RITA LEIBINGER for the best biocompatibility.



## Anatomically Shaped Limited Contact Dynamic Compression Plates

The LeiLOX CBLO plates are contoured to match the anatomic shape of the bone. This makes it easier to place the plate in an optimal position.

The plate features limited contact dynamic compression to minimize vascular damage to the plated bone segment.



## Double Compression

Two precisely designed compression holes enable a very tight compression of the osteotomy. This allows you to use a standard cortical screw as the cranio-caudal holding screw (instead of a headless compression screw).



## Interchangeable 2.0/2.4 & 2.7/3.5mm Screws

Because the screwheads are identical, all Titanium 2.7/3.5 LeiLOX plates (TPLO Swing, CBLO, and CCWO systems) work with 2.7mm as well as 3.5mm screws in all of the plate sizes. Same applies for the 2.0/2.4 systems. This offers flexibility and ideal implant selection for each patient. Moreover, this saves on inventory cost.

High Performance Sawblades are available. The Titanium Nitrate coating allows them to last significantly longer than standard blades.

# LeiLOX

**CBLO** Locking System



Special Thanks to  
Dr. Hugo Schmökel

## LeiLOX CBLO

**R** RITA  
LEIBINGER  
MEDICAL

# LEILOX CBLO TECHNIQUE

## Pre-Operative Planning

### Positioning the Patient for Radiographs

Proper positioning is essential for accurate planning. Orthogonal radiographs are taken with the stifle positioned at 90 degrees and the tarsus at 90 degrees for the lateral projection. The AP projection must have the stifle and tarsus included for the attending surgeon to assess limb alignment. The patient is best sedated for radiographs to assure optimal positioning.

### Determining the CORA

The distal mid-diaphyseal line (FA) as well as the Tibia Plateau (TP) are determined.



The proximal axis (PA) is determined from the intersection point on the tibia plateau with the angle  $\alpha$  [normally  $80^\circ = 90^\circ - 10^\circ$  (post-operative required TP angle)].

The intersection point of FA and PA is the **CORA**.

The angle  $\beta$  is then the correction.

The required saw blade is determined by a circle CORA as the centre point. Draw and measure a line (D1) from the insertion of the patella tendon to the point at which the saw blade crosses the cranial cortex. Draw and measure a second line (D2) from the joint line at a point where the MCL crosses the joint to the location where the saw blade crosses the caudal cortex. With these D1 and D2 measurements, the osteotomies can be positioned correctly during the surgery.

### Determining the Correction

Based on the measured correction angle and the selected saw blade select the appropriate correction in the Leibinger LeiLOX CBLO Rotation Chart in the field "Rotation".

View or Download the rotation chart here



### LeiLOX CBLO Rotation Chart

Correction Angle		5°	6°	7°	8°	9°	10°	11°	12°	13°	14°	15°	16°	17°	18°	19°	20°	21°	22°	23°	24°	25°	26°	27°	28°	29°	30°	31°	32°	33°	34°
Radians		0.04	0.05	0.06	0.07	0.08	0.09	0.10	0.10	0.11	0.12	0.13	0.14	0.15	0.16	0.17	0.17	0.18	0.19	0.20	0.21	0.22	0.23	0.24	0.24	0.25	0.26	0.27	0.28	0.29	0.30
Saw blade	9mm	0.8	0.9	1.1	1.3	1.5	1.6	1.7	1.9	2.1	2.2	2.4	2.5	2.7	2.8	3.0	3.2	3.3	3.5	3.6	3.8	3.9	4.1	4.2	4.4	4.5	4.7	4.8	5.0	5.1	5.3
	12mm	1.0	1.3	1.5	1.7	1.9	2.1	2.3	2.5	2.7	2.9	3.1	3.3	3.5	3.8	4.0	4.2	4.4	4.6	4.8	5.0	5.2	5.4	5.6	5.8	6.0	6.2	6.4	6.6	6.8	7.0
	15mm	1.3	1.6	1.8	2.1	2.4	2.6	2.9	3.1	3.4	3.7	3.9	4.2	4.4	4.7	5.0	5.2	5.5	5.7	6.0	6.2	6.5	6.7	7.0	7.3	7.5	7.8	8.0	8.3	8.5	8.8
	18mm	1.6	1.9	2.2	2.5	2.8	3.1	3.5	3.8	4.1	4.4	4.7	5.0	5.3	5.6	5.9	6.3	6.6	6.9	7.2	7.5	7.8	8.1	8.4	8.7	9.0	9.3	9.6	9.9	10.2	10.5
	21mm	1.8	2.2	2.6	2.9	3.3	3.7	4.0	4.4	4.8	5.1	5.5	5.8	6.2	6.6	6.9	7.3	7.7	8.0	8.4	8.7	9.1	9.4	9.8	10.2	10.5	10.9	11.2	11.6	11.9	12.3
	24mm	2.1	2.5	2.9	3.3	3.8	4.2	4.6	5.0	5.4	5.8	6.3	6.7	7.1	7.5	7.9	8.3	8.7	9.2	9.6	10.0	10.4	10.8	11.2	11.6	12.0	12.4	12.8	13.2	13.6	14.0
	27mm	2.4	2.8	3.3	3.8	4.2	4.7	5.2	5.6	6.1	6.6	7.0	7.5	8.0	8.4	8.9	9.4	9.8	10.3	10.8	11.2	11.7	12.1	12.6	13.1	13.5	14.0	14.4	14.9	15.3	15.8
	30mm	2.6	3.1	3.7	4.2	4.7	5.2	5.8	6.3	6.8	7.3	7.8	8.4	8.9	9.4	9.9	10.4	10.9	11.4	12.0	12.5	13.0	13.5	14.0	14.5	15.0	15.5	16.0	16.5	17.0	17.5
	33mm	2.9	3.5	4.0	4.6	5.2	5.8	6.3	6.9	7.5	8.0	8.6	9.2	9.8	10.3	10.9	11.5	12.0	12.6	13.2	13.7	14.3	14.8	15.4	16.0	16.5	17.1	17.6	18.2	18.7	19.3

## Surgery Protocol

### Positioning of the Patient

The dog is placed in a dorsal recumbency with the affected limb suspended from a stand. Make sure that the dog's paws are not fixed too tightly, since the affected limb will be put against the table later in the surgery. CBLO is performed through a medial skin incision. The internal structures of the joint should be examined, this is accomplished arthroscopically or with a medial open mini arthrotomy.

Most importantly, the caudal horn of the medial meniscus must be examined closely and torn meniscus parts excised if present. Next, the insertion of the sartorius muscle is reflected from the medial tibia to expose the MCL. Limited reflection of the popliteal muscle and protection of the popliteal artery with gauze packing or Hohmann retractor is optional. D1 and D2 measurements are marked distal to the insertion of the patella tendon (D1) and distal to the joint line at the MCL (D2).



**Use of a Jig**

The use of a jig is advised when performing a leveling osteotomy.

### Placement of the Jig

The proximal pin of the jig is inserted about 3-4mm below the joint surface caudal to the MCL. The pin must be absolutely parallel to the joint surface.



The Jig is slid over the proximal pin. The Jig can be used as a guide for placing the distal pin. Both pins must be parallel to each other. The Jig must be in a right angle to the pins. After the positions are correct, the screws as well as the grub screws can be tightened.

### Making the Osteotomy


- 1 The appropriate saw blade determined in the pre-operative planning is positioned at D1/D2 and a circular osteotomy begins. The osteotomy is stopped when 1/3 to 1/2 complete. Move the saw circularly so that it won't stick. The pre-operatively determined correction measurements (in mm) should be marked for example by a small chisel and mallet.
- 2 At the insertion point of the patella a 2.0mm pin can be preplaced without crossing the osteotomy.



- 3 Complete the cut and rotate the bone fragment. The rotation is made with the pin so that the marks are aligned. The osteotomy is then stabilized with the pin. Carefully avoid a rotation or valgus mistake. The preplaced pin is directed across the osteotomy under the medial cortex to exit the caudal cortex of the tibia distal to the osteotomy.

### Stabilization of the Osteotomy with Plate Compression

The CBLO procedure not only levels the tibial plateau, but also involves cranially advancing the tibial crest. This advancement enhances the structural moment arm of the tibia, consequently increasing quadriceps force on the osteotomy site. To increase



stability and promote faster healing, compression of the osteotomy is essential.

The LeiLOX CBLO plate facilitates this compression, particularly when the distal portion of the plate sits flush on the tibial surface without exerting lateral pressure on

the proximal tibia. By positioning the LeiLOX CBLO Plate at the desired location and pre-fixing it with a 1mm positioning pin in the plate shaft, precise compression and stabilization of the osteotomy can be achieved.


Original Author (English version):  
Dr. Hugo Schmökel, Dr.med.vet. PhD, Dipl. ECVS



**cblo.leibinger.vet**

### Sequence of Screw Insertion

The screws are inserted in the following (recommended) sequence:

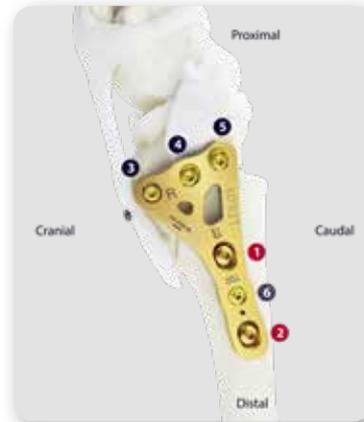

- 1 2 The first screws to be placed are the **2 cortical screws** in the 2 compression holes in the plate. Drill the holes with the matching compression drill guide facing distal. Place the screw but do not tighten yet.

- 3 4 5

Place the proximal **locking screws** in the plate head. Drill the hole with the matching locking drill guide and insert the screw one by one. Fully tighten the screws.

*NOTE: The locking mechanism of the LeiLOX CBLO plate is designed multi-axial, offering versatility and adaptability during surgical procedures. If there is concern about screws entering the joint when drilling at a 90° angle, simply adjust the angle of the drill guide to face distally. This adjustment allows for precise screw placement while minimizing the risk of intra-articular penetration.*

Remove the stabilizing pin and the positioning pin.

- 1 2

Tighten the compression screws 1 and 2.

- 6

Insert **locking screw 6** and tighten.



#### Screws

To counteract the pull of the quadriceps muscle, a screw should be placed in the same location as the pin through the crest in a caudo-distal direction.



In large dogs it is advised to place 2 cranial screws to counteract the quadriceps force. In giant breed dogs the placement of a second plate should be considered.

*Image: Big dogs, stabilized with a 3.5mm broad plate and two cranial screw*

Check the tightness of all screws.

Close the wound using standard techniques. It is crucial to properly close the periosteum and soft tissue layers to safeguard the plate site. Ensure not to overlook the closure of incision made for the distal jig pin.

**2.0 / 2.4 LeiLOX CBLO Set**

Contents:

- 1 CBLO Implants and Instruments Tray with Lid
- 2 of each CBLO Plate
- 3 of each Cortical Screw (8-18mm // 8-22mm, 42 total)
- 5 of each Locking Screw (6-24mm // 6-30mm, 115 total)
- 2 Drills (1.5 & 1.8mm)
- 5 K-Wires
- 2x2 Locking Drill Guides
- 2 Compression Drill Guides
- 1 TPLO Jig
- 1 Screwdriver Handle
- 1 Screwdriver Shaft T8
- 1 Depth Gauge



**142-4200-00**

Tray without contents

**142-4200-10**



**Sterilization Container**

See Sterilization Containers for Implants and Instruments Trays on **Page 204**.

**2.0 / 2.4 LeiLOX CBLO Locking Plates**



LeiLOX CBLO Locking Plate, 2.0 mm, left, 35 mm, titanium

**142-2320-10**



LeiLOX CBLO Locking Plate, 2.0 mm, right, 35 mm, titanium

**142-2320-00**



LeiLOX CBLO Locking Plate, 2.4 mm, left, 40 mm, titanium

**142-2324-10**



LeiLOX CBLO Locking Plate, 2.4 mm, right, 40 mm, titanium

**142-2324-00**

## CBLO Screws Locking & Non-Locking 2.0/2.4 Titanium

### 2.0 / 2.4 LeiLOX Locking Screw Titanium

For LeiLOX Locking Systems, LeiStar T8  
self-holding (T8 Shaft from Rita Leibinger recommended)  
self-tapping with three flute cutting edge



	2.0 mm	2.4 mm
Length (mm)	Product Code	Product Code
06	242-220-06	242-224-06
08	242-220-08	242-224-08
10	242-220-10	242-224-10
12	242-220-12	242-224-12
14	242-220-14	242-224-14
16	242-220-16	242-224-16
18	242-220-18	242-224-18
20	242-220-20	242-224-20
22	242-220-22	242-224-22
24	242-220-24	242-224-24
26	242-220-26	242-224-26
28	242-220-28	242-224-28
30	242-220-30	242-224-30
32		242-224-32
34		242-224-34
36		242-224-36
38		242-224-38
40		242-224-40

### 2.0 / 2.4 Cortical Screw (Non-Locking) Titanium

LeiStar T8, Non-Locking  
self-holding (T8 Shaft from Rita Leibinger recommended)  
self-tapping with three flute cutting edge



	2.0 mm	2.4 mm
Length (mm)	Product Code	Product Code
08	245-520-08	245-524-08
10	245-520-10	245-524-10
12	245-520-12	245-524-12
14	245-520-14	245-524-14
16	245-520-16	245-524-16
18	245-520-18	245-524-18
20		245-524-20
22		245-524-22

See more screw lengths on **Page 126.**

Screw Racks on **Page 198.**

**2.7 / 3.5 LeiLOX CBLO Set**

Contains:

- 1 CBLO Implants and Instruments Tray with Lid
- 1 Screwcrack CBLO 2.7
- 1 Screwcrack CBLO 3.5
- 2 of each CBLO Plate
- 3 of each 2.7mm Cortical Screw (16-34mm)
- 3 of each 3.5mm Cortical Screw (16-34mm)
- 5 of each 2.7mm Locking Screw (16-46mm)
- 5 of each 3.5mm Locking Screw (16-60mm)



**142-4000-10**

Tray without contents

**142-4000-01**



**2.7 / 3.5 LeiLOX CBLO Locking Plates**



LeiLOX CBLO Plate, 2.7 mm, left, 55 mm, titanium

**142-2327-10**



LeiLOX CBLO Plate, 2.7 mm, right, 55 mm, titanium

**142-2327-00**



LeiLOX CBLO Plate, 3.5 mm, left, 70 mm, titanium

**142-2335-10**



LeiLOX CBLO Plate, 3.5 mm, right, 70 mm, titanium

**142-2335-00**



LeiLOX CBLO Plate, broad, 3.5 mm, left, 78 mm, titanium

**142-2335-60**



LeiLOX CBLO Plate, broad, 3.5 mm, right, 78 mm, titanium

**142-2335-50**

## CBLO Screws Locking & Non-Locking 2.7/3.5 Titanium

### 2.7 / 3.5 LeiLOX Locking Screw Titanium

For LeiLOX Locking Systems, LeiStar T10 self-holding (T10 Shaft from Rita Leibinger recommended) self-tapping with three flute cutting edge



	2.7 mm	3.5 mm
Length (mm)	Product Code	Product Code
10	242-227-10	242-235-10
12	242-227-12	242-235-12
14	242-227-14	242-235-14
16	242-227-16	242-235-16
18	242-227-18	242-235-18
20	242-227-20	242-235-20
22	242-227-22	242-235-22
24	242-227-24	242-235-24
26	242-227-26	242-235-26
28	242-227-28	242-235-28
30	242-227-30	242-235-30
32	242-227-32	242-235-32
34	242-227-34	242-235-34
36	242-227-36	242-235-36
38	242-227-38	242-235-38
40	242-227-40	242-235-40
42	242-227-42	242-235-42
44	242-227-44	242-235-44
46	242-227-46	242-235-46
48	242-227-48	242-235-48
50	242-227-50	242-235-50
52		242-235-52
54		242-235-54
56		242-235-56
58		242-235-58
60		242-235-60

### 2.7 / 3.5 Cortical Screw Titanium

LeiStar T10, Non-Locking self-holding (T10 Shaft from Rita Leibinger recommended) self-tapping with three flute cutting edge



	2.7 mm	3.5 mm
Length (mm)	Product Code	Product Code
16	245-527-16	245-535-16
18	245-527-18	245-535-18
20	245-527-20	245-535-20
22	245-527-22	245-535-22
24	245-527-24	245-535-24
26	245-527-26	245-535-26
28	245-527-28	245-535-28
30	245-527-30	245-535-30
32	245-527-32	245-535-32
34	245-527-34	245-535-34




#### TPLO Saw Blades

See radial saw blades for TPLO and CBLO in various radii on [Page 191](#).




#### Screw Racks

See screw racks for 1.5mm up to 3.5mm screws on [Page 198](#).



#### CBLO Instruments

See essential instruments for a CBLO Surgery on [Page 78](#).



#### Instrument Set

See Instrument Set for TPLO / CBLO / CCWO on [Page 78](#).

See more screw lengths on [Page 126](#).

# LeiLOX CCWO



## Advantages of CCWO

Straightforward technique through linear cuts. Suitable for juvenile patients as the procedure is carried out outside the growth zone. Moreover, it is suitable for patients with steep TPAs that would be too challenging to treat with other techniques.



## Multiaxial Locking

The screws can be locked in a 90° angle with a 12° deviation in any direction. This allows screws to be angled away from vital structures, providing greater flexibility in fixation. The robust LeiStar screw head can be locked firmly into the plate.



## Anatomically Shaped Limited Contact Dynamic Compression Plates

The LeiLOX CCWO plates are contoured to match the natural shape of the bone. It simplifies placement of the plate in an optimal position and provides high stability.

The plate features limited contact dynamic compression to minimize vascular damage to the plated bone segment, promoting better blood flow and faster healing.



## Titanium for Best Biocompatibility

LeiLOX CCWO implants are made of medical grade Titanium, offering several key advantages: it is biocompatible, ensuring it is well-tolerated by the body and reducing the risk of adverse reactions; it provides strength and durability, offering robust support during the bone healing process and ensuring long-term stability; and it is resistant to corrosion, making it suitable for long-term implantation and maintaining its integrity over time.

## Interchangeable 2.7 & 3.5mm and 2.0 & 2.4mm Screws

Because the screwheads are identical, all Titanium 2.7/3.5 LeiLOX plates (TPLO Swing, CBLO, and CCWO systems) work with 2.7mm as well as 3.5mm screws in all of the plate sizes. Same applies for the 2.0/2.4 systems. This offers flexibility and ideal implant selection for each patient. Moreover, this saves on inventory cost.



High Performance Sawblades are available. The Titanium Nitrate coating allows them to last significantly longer than standard blades.

# LeiLOX

**CCWO** Locking System



LeiLOX **CCWO**

**R** **RITA**  
**LEIBINGER**  
MEDICAL

## LEILOX CCWO TECHNIQUE

### Pre-Operative Planning

#### Positioning the Patient for Radiographs

Proper positioning is essential for accurate planning. By ensuring proper positioning of the limb, accurate radiographs with consistent appearance of anatomic landmarks can be obtained for CCWO (Cranial Closing Wedge Osteotomy) pre-operative planning, allowing for precise measurements.

To obtain lateral radiographic views of the stifle joint and tibia, the patient is positioned in lateral recumbency on a radiographic table, with the stifle and tarsus positioned at 90°. The patient is best sedated to ensure optimal positioning. Orthogonal radiographs are taken with the beam centered over the stifle joint.

It is important to know that any internal or external rotation of the tibia can affect how the tibial plateau appears on the X-ray. This rotation can occur due to incorrect positioning of the affected limb or not centering the X-ray beam accurately over the stifle joint.

#### Determining the Tibial Plateau Angle (TPA)



**Draw the functional axis (FA),** also known as the weight bearing axis or mechanical tibial axis. Draw a line from the intercondylar eminence or tibial eminence proximally to the center of the tarsal joint or talocrural joint distally.

**Draw the tibial plateau line (TP).** To check correctness of the tibial plateau line, the cranial and caudal points of this line should be equally distant from the intercondylar eminence.

Draw a line perpendicular to the FA, where it intersects with the TP. The **TPA** is the angle between this line and TP.


There are several CCWO Techniques in achieving the target TPA. The following procedure aims for a post-operative TPA of 5°.

#### Draw the Mid-Diaphyseal Line (A)



The proximal mid-diaphyseal line bisects the marrow cavity at the distal extent of the tibial crest and 1-2 cm below; it generally exits the joint line at Gerdy's tubercle. To help visualize the anatomic tibia axis, see image of an intramedullary pin at the left.


#### Determining Wedge Size and Position

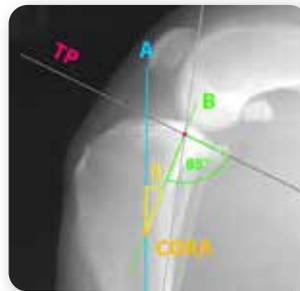

Draw a proximal axis line (**B**) from the intersection point of TP and FA at an angle of 85°, intersecting it with the mid-diaphyseal line (**A**). The intersection point of these two lines is the **CORA**.



Angle  $\beta$  is the correction angle. Next, the proximal wedge line is drawn from the cranial to the caudal cortex through the CORA. The distal wedge line is drawn from the CORA at the correction angle  $\beta$  to the cranial cortex.

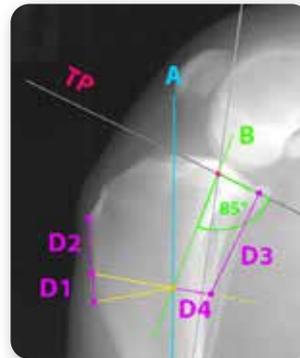

Note down the following measurements:

- D1** - from the insertion point of the patellar tendon to the cranial exit point of the proximal osteotomy
- D2** - distance between exit points of the cranial proximal and distal osteotomies
- D3** - from the caudal cortex to the caudal end of the tibia
- D4** - from the CORA to the caudal cortex

### Surgery Protocol

#### Positioning of the Patient

The dog is placed in a dorsal recumbency with the affected limb suspended from a stand. Make sure that the dog's paws are not fixed too tightly, since the affected limb will be put against the table later in the surgery. CCWO is performed through a medial skin incision.



#### Use of a Jig

The use of a jig is advised when performing a CCWO.

#### Placement of the Jig

- 1 The joint surface is marked with a needle. About 3 to 4 mm below is the insertion point of the proximal pin for the TPLO Jig.
- 2 The proximal pin is inserted in a 90° angle to the joint surface.
- 3 The distal pin is placed. Take care to not tilt the jig. The pins must be parallel to each other, and absolutely perpendicular to the jig.

## LEILOX CCWO TECHNIQUE



### Making the Osteotomy

- 1 With the measurements D1, D2, D3, and D4 determined during pre-op planning, mark the angle for the wedge cut. Use a wedge osteotomy gauge if needed. The cutting line can be outlined using an electrocautery device.
- 2 Holes for the cerclage proximal and distal to the wedge may already be made before the osteotomy.
- 3 Using a sagittal saw, perform the osteotomy, making sure that the cut aligns with the pins.
- 4 The wedge is removed and the proximal bone fragment is rotated to close the wedge. A cerclage may be placed to close the osteotomy. Ensure that the bone fragments do not move relative to each other.
- 5 If necessary, place a holding pin, or fix the plate straight away.



### Placement of the CCWO Plate

Place the CCWO Plate, securing it in place with K-Wires. The screws are inserted in the following (recommended) sequence:



1

Prepare the hole in the bone for the cortical screw. Use the drill guide in compression position. Insert the **cortical screw 1** into the compression hole. Do not tighten yet.



**TIP:** Use a depth gauge to determine the required length of the screws and add about 2-3mm to the measure.



2 3 4

Drill the holes with the matching locking drill guide and insert **locking screws 2, 3, and 4** one by one. Fully tighten the screws.



The locking mechanism of the LeiLOX CCWO plate is designed to be multi-axial. If there is a risk of the screws ending in the joint when drilling in a 90° angle, simply adjust the angle of the drill guide to face distally.

*NOTE: We recommend that the jig be removed only when at least 2 screws have already been fixed into the plate.*



1

Tighten compression screw 1 in the compression hole to reduce the osteotomy.



5 6

Insert remaining **locking screws 5 and 6** and tighten.

Check the tightness of all screws. Close the wound using standard techniques. It is crucial to properly close the periosteum and soft tissue layers to safeguard the plate site. Ensure not to overlook the closure of incision made for the distal jig pin.

Author: **Dr. Hugo Schmökel**, DVM, PhD, Dipl. ECVS, MRCVS

**2.0 / 2.4 CCWO Set**

Contains:

- 1 CCWO Implants and Instruments Tray with Lid
- 2 of each CCWO Locking Plate
- 3 of each Cortical Screw (2.0, 8-18mm // 2.4, 8-22mm, 42 total)
- 5 of each Locking Screw (2.0, 6-24mm // 2.4, 6-30mm, 115 total)
- 2 Drills (1.5 & 1.8mm)
- 5 K-Wires
- 2x2 Locking Drill Guides
- 2 Compression Drill Guides
- 1 TPLO Jig
- 1 Screwdriver Handle
- 1 Screwdriver Shaft T8
- 1 Depth Gauge



**142-2920-24**

Tray without contents

**142-2900-10**



**Sterilization Container**

See Sterilization Containers for Implants and Instruments Trays on **Page 204**.

**2.0 / 2.4 LeiLOX CCWO Locking Plates Titanium**



LeiLOX CCWO Locking Plate  
2.0 mm, left, 33 mm, Titanium

**142-2920-10**



LeiLOX CCWO Locking Plate  
2.0 mm, right, 33 mm, Titanium

**142-2920-00**



LeiLOX CCWO Locking Plate  
2.4 mm, left, 37 mm, Titanium

**142-2924-10**



LeiLOX CCWO Locking Plate  
2.4 mm, right, 37 mm, Titanium

**142-2924-00**

## CCWO Screws Locking & Non-Locking 2.0/2.4 Titanium

### 2.0 / 2.4 LeiLOX Locking Screw Titanium

For LeiLOX Locking Systems, LeiStar T8  
self-holding (T8 Shaft from Rita Leibinger recommended)  
self-tapping with three flute cutting edge



	2.0 mm	2.4 mm
Length (mm)	Product Code	Product Code
06	242-220-06	242-224-06
08	242-220-08	242-224-08
10	242-220-10	242-224-10
12	242-220-12	242-224-12
14	242-220-14	242-224-14
16	242-220-16	242-224-16
18	242-220-18	242-224-18
20	242-220-20	242-224-20
22	242-220-22	242-224-22
24	242-220-24	242-224-24
26	242-220-26	242-224-26
28	242-220-28	242-224-28
30	242-220-30	242-224-30
32		242-224-32
34		242-224-34
36		242-224-36
38		242-224-38
40		242-224-40

### 2.0 / 2.4 Cortical Screw (Non-Locking) Titanium

LeiStar T8, Non-Locking  
self-holding (T8 Shaft from Rita Leibinger recommended)  
self-tapping with three flute cutting edge



	2.0 mm	2.4 mm
Length (mm)	Product Code	Product Code
08	245-520-08	245-524-08
10	245-520-10	245-524-10
12	245-520-12	245-524-12
14	245-520-14	245-524-14
16	245-520-16	245-524-16
18	245-520-18	245-524-18
20		245-524-20
22		245-524-22

See more screw lengths on **Page 126.**

Screw Racks on **Page 198.**



[ccwo.leibinger.vet](https://ccwo.leibinger.vet)

LEARN FROM THE BEST

### WORKSHOPS

Learn the CCWO Technique  
in one of our workshops.

[academy.leibinger.vet](https://academy.leibinger.vet)


**2.7 / 3.5 CCWO Set**

- Contains:
- 1 CCWO Implant Tray with Lid
- 2 of each CCWO Plate  
(2.7, 3.5, 3.5 broad)
- 3 of each Cortical Screw  
(16-34mm, 60 total)
- 5 of each Locking Screw  
(16-46mm, 160 total)

**142-2927-35**

Tray without contents

**142-2900-20**

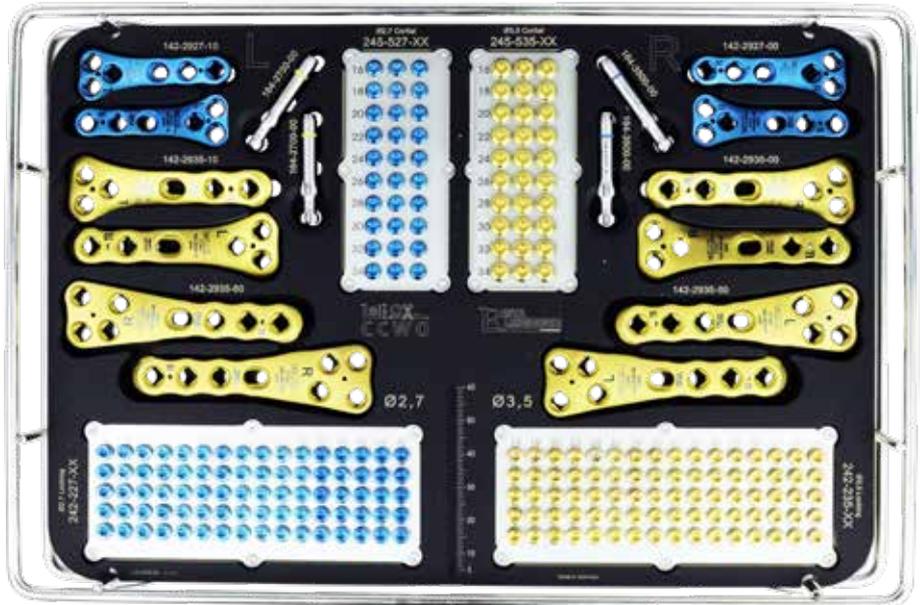

**2.7 / 3.5 LeiLOX CCWO Locking Plates Titanium**



LeiLOX CCWO Locking Plate  
2.7 mm, left, 44 mm, Titanium

**142-2927-10**



LeiLOX CCWO Locking Plate  
2.7 mm, right, 44 mm, Titanium

**142-2927-00**



LeiLOX CCWO Locking Plate  
3.5 mm, left, 63 mm, Titanium

**142-2935-10**



LeiLOX CCWO Locking Plate  
3.5 mm, right, 63 mm, Titanium

**142-2935-00**



LeiLOX CCWO Locking Plate  
3.5 mm, left, 74 mm, Titanium

**142-2935-60**



LeiLOX CCWO Locking Plate  
3.5 mm, right, 74 mm, Titanium

**142-2935-50**

## CCWO Screws Locking & Non-Locking 2.7/3.5 Titanium

### 2.7 / 3.5 LeiLOX Locking Screw Titanium

For LeiLOX Locking Systems, LeiStar T10 self-holding (T10 Shaft from Rita Leibinger recommended) self-tapping with three flute cutting edge



	2.7 mm	3.5 mm
Length (mm)	Product Code	Product Code
10	242-227-10	242-235-10
12	242-227-12	242-235-12
14	242-227-14	242-235-14
16	242-227-16	242-235-16
18	242-227-18	242-235-18
20	242-227-20	242-235-20
22	242-227-22	242-235-22
24	242-227-24	242-235-24
26	242-227-26	242-235-26
28	242-227-28	242-235-28
30	242-227-30	242-235-30
32	242-227-32	242-235-32
34	242-227-34	242-235-34
36	242-227-36	242-235-36
38	242-227-38	242-235-38
40	242-227-40	242-235-40
42	242-227-42	242-235-42
44	242-227-44	242-235-44
46	242-227-46	242-235-46
48	242-227-48	242-235-48
50	242-227-50	242-235-50
52		242-235-52
54		242-235-54
56		242-235-56
58		242-235-58
60		242-235-60

See more screw lengths on **Page 126**.

### 2.7 / 3.5 Cortical Screw Titanium

LeiStar T10, Non-Locking self-holding (T10 Shaft from Rita Leibinger recommended) self-tapping with three flute cutting edge



	2.7 mm	3.5 mm
Length (mm)	Product Code	Product Code
16	245-527-16	245-535-16
18	245-527-18	245-535-18
20	245-527-20	245-535-20
22	245-527-22	245-535-22
24	245-527-24	245-535-24
26	245-527-26	245-535-26
28	245-527-28	245-535-28
30	245-527-30	245-535-30
32	245-527-32	245-535-32
34	245-527-34	245-535-34




#### Saw Blades

See saw blades for CCWO on **Page 190**.




#### Screw Racks

See screw racks for 1.5mm up to 3.5mm screws on **Page 198**.



#### CCWO Instruments

See essential instruments for a CCWO Surgery on **Page 78**.



#### Instrument Set

See Instrument Set for TPLO / CBLO / CCWO on **Page 78**.

# LeiLOX INSTRUMENTS



# LeILOX

**TPLO** | **CBLO** | **CCWO**




## INSTRUMENTS

**R** **RITA**  
**LEIBINGER**  
MEDICAL

**TPLO/CBLO/CCWO Instrument Set**

Contains:

- 1 CBLO Instrument Tray
- 2 Drills (2.0 & 2.5mm)
- 3x2 K-Wires (1.0, 2.5 & 3.0mm)
- 2x2 Locking Drill Guides
- 2 TPLO Jigs
- 1 Screwdriver Handle
- 1 Screwdriver Shaft
- 1 Depth Gauge
- 1 Castroviejo Caliper
- 2 Compression Drill Guides

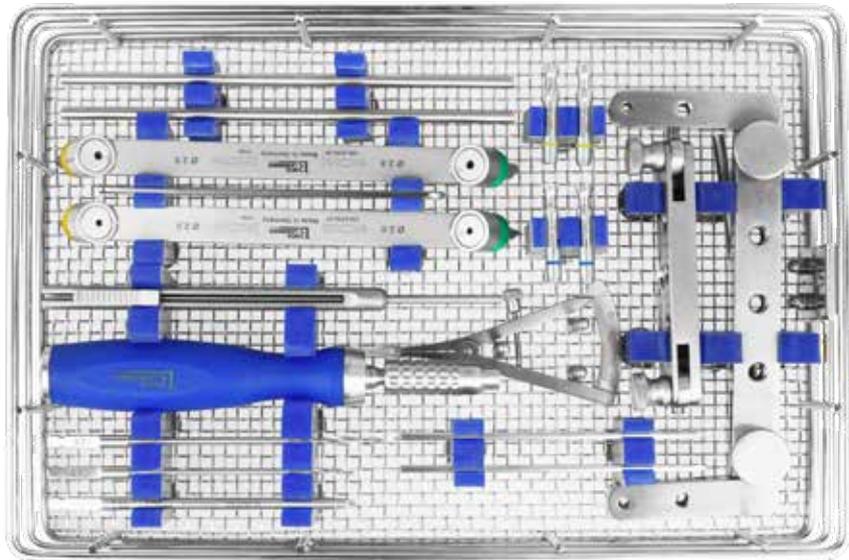

**142-0100-01**

Tray without contents

**142-0100-20**



**Sterilization Container**

See Sterilization Containers for Implants and Instruments Trays on **Page 204**.

**TPLO/CBLO/CCWO Jig**

Product Code	Description
<b>128-4354-00</b>	for 2.0/2.4 mm
<b>128-4355-00</b>	for 2.7 mm
<b>128-4356-00</b>	for 3.5 mm



**Castroviejo**

Caliper

**17-3105-08**



## Depth Gauge

## Compression Drill Guide

## Locking Drill Guide

## Depth Gauge



Product Code	Description	Compatibility
164-1520-20	150mm in length, scale up to 40mm	for 1.5/2.0/2.4 mm screws
164-2735-60	150mm in length, scale up to 60mm	for 2.4/2.7/3.5 mm screws

## Compression Drill Guide

Neutral / Load



Product Code	Description
164-0071-15	for screws Ø 2.0 mm and drills Ø 1.5 mm
128-2418-24	for screws Ø 2.4 mm and drills Ø 1.8 mm
128-2720-27	for screws Ø 2.7 mm and drills Ø 2.0 mm
128-2535-35	for screws Ø 3.5 mm and drills Ø 2,5mm

## Locking Drill Guide

Stainless Steel

Product Code	Description
164-2000-00	for 2.0 mm screws
164-2400-00	for 2.4 mm screws
164-2700-00	for 2.7 mm screws
164-3500-00	for 3.5 mm screws



## K-Wire

 Single Trocar  
 1.0 mm x 100 mm

Product Code	Dimensions (mm)
144-1010-10	1.0 x 100
144-1020-10	2.0 x 100
144-1025-10	2.5 x 100
144-1030-10	3.0 x 100


 See more K-Wires on **Page 136.**

Twist Drill



Product Code	Ø (mm)	for Screw Ø (mm)	Length (mm)	Connection
148-0080-15	1.5	for 2.0 screws	70	round shaft
148-0080-18	1.8	for 2.4 screws	125	round shaft
148-0080-20	2.0	for 2.7 screws	85	round shaft
148-0080-25	2.5	for 3.5 screws	95	round shaft



Product Code	Ø (mm)	for Screw Ø (mm)	Length (mm)	Connection
148-0081-15	1.5	for 2.0 screws	85/60	AO QC
148-0081-18	1.8	for 2.4 screws	125/25	AO QC
148-0081-20	2.0	for 2.7 screws	100/75	AO QC
148-0081-25	2.5	for 3.5 screws	110/85	AO QC

See more on **Page 199.**

Screwdriver Shaft LeiStar

AO connection, self-holding



Product Code	Description
128-2024-08	T8 for 2.0 / 2.4 mm screws, 100 mm in length
128-2735-10	T10 for 2.7 / 3.5 mm screws, 100 mm in length

See more Screwdriver Shafts on **Page 200.**

Screwdriver Handle

Silicone, AO-Connection  
sterilizable up to 134°C / 273°F



Product Code	Description
247-0103-00	compact, compatible with 2.7/3.5
247-0102-00	standard, compatible with 2.7/3.5

Torque Limiting Screwdriver Handle

Torque 3 Nm  
Silicone, AO, sterilizable up to 134°C / 273°F



247-0104-00

## Radiography Calibration Ball

### Radiography Calibration Ball


Flexible arm, Stainless Steel 25mm Ø Reference Ball and base plate

**100-2000-25**



#### **TPLO Saw Blades**

See radial saw blades for TPLO and CBLO in various radii on **Page 191.**



#### **Saw Blades**

See saw blades for CCWO on **Page 190.**



#### **Power Tools**


See power tools and attachments on **Page 186.**

# LeiLOX 1.0/1.3 Nano



## Titanium Locking Fracture System for the smallest patients

Introducing our new LeiLOX 1.0/1.3 Titanium Locking Plate System, specially developed for the smallest patients and bones, such as toy breeds, rodents, or birds.

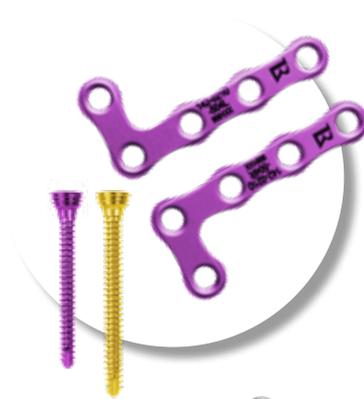

## Titanium: Best Biocompatibility

Made of medical-grade Titanium, these implants are lightweight yet strong, minimizing stress on tiny bones. The high biocompatibility lowers the risk of infections. Furthermore, titanium's flexibility allows for precise and delicate fracture fixation, making it the ideal choice for the most fragile patients.



## All-in-One Set

The new LeiLOX 1.0/1.3 Set provides everything you need to treat fractures in the tiniest patients. It includes a range of plates from standard to various unique shapes to accommodate complex anatomies. Additionally, the set comes with all the essential instruments you may require, ensuring you are fully equipped to handle even the most delicate fracture cases.



## Various Applications

With 24 different plates, LeiLOX 1.0/1.3 is the perfect solution to treat a wide variety of fracture cases: Y-Plates, L-Plates, Bridge-Plates, Standard-Plates, Cuttable 20-hole Plates and many Challenger Plates offer plenty of possibilities: from maxillofacial and pelvic fractures, to the fixation of long tubular bones.

## LeiStar Screws

All of our locking screwheads are LeiStar, which allows for best tightening torque. Additionally, the screws provide a self-holding feature when used with a RITA LEIBINGER screwdriver shaft, keeping the screws securely on the driver.



# LeiLOX

1.0/1.3 NanoLocking System



LeiLOX 1.0/1.3 NANO

**R** RITA  
LEIBINGER  
MEDICAL

## LeiLOX Locking Set 1.0/1.3 Titanium

### 1.0/1.3 Osteosynthesis Locking Set Titanium

Contains:

- 1 Tray for Implants and Instruments with Lid
- 1 Locking Plate of each style (24 pcs. total)
- 5 of each 1.0 Locking Screw (4-20mm, 65 pcs. total)
- 5 of each 1.3 Locking Screw (4-20mm, 65 pcs. total)
- 1 Screwdriver Shaft T5
- 1 Screwdriver Handle
- 2x2 Locking Drill Guides, 1.0 & 1.3
- 1 Depth Gauge
- 2 Drills (AO, 0.7 & 1.0)
- 1 pair of Bending Irons

**142-1013-00**

Tray without contents

**142-1013-10**

**NEW**



#### Sterilization Container

See Sterilization Containers for Implants and Instruments Trays on **Page 204**.

### 1.0 Locking Plate Titanium

3.5 mm wide, 1.0 mm thick



Product Code	Description
<b>142-0210-04</b>	4-Hole, 18.5 mm
<b>142-0210-05</b>	5-Hole, 23.5 mm
<b>142-0210-06</b>	6-Hole, 28.5 mm
<b>142-0210-07</b>	7-Hole, 33.5 mm
<b>142-0210-08</b>	8-Hole, 38.5 mm
<b>142-0210-09</b>	9-Hole, 43.5 mm
<b>142-0210-10</b>	10-Hole, 48.5 mm
<b>142-0210-20</b>	20-Hole, 98.5 mm, cuttable

### 1.0 Locking Plate with Bridge, Titanium

3.5 mm wide, 1.0 mm thick



Product Code	Description
<b>142-0210-610</b>	10 mm Bridge, 4-Hole, 23.5mm
<b>142-0210-615</b>	15 mm Bridge, 6-Hole, 38.5mm
<b>142-0210-625</b>	25 mm Bridge, 6-Hole, 48.5mm
<b>142-0210-633</b>	33 mm Bridge, 6-Hole, 56.5 mm
<b>142-0210-643</b>	43 mm Bridge, 6-Hole, 66.5 mm

### 1.0 Locking-L-Plate Titanium

3.5 mm / 8.5 mm wide, 1.0 mm thick, 18.5 mm long



Product Code	Description
<b>142-0210-504L</b>	left
<b>142-0210-504R</b>	right

### 1.0 T-Locking Plate Titanium

3.5 mm wide, 1.0 mm thick, cuttable



Product Code	Description
<b>142-0210-38</b>	1.0 mm, 3/8-Hole, 46 mm
<b>142-0210-49</b>	1.0 mm, 4/8-Hole, 47 mm

LeiLOX Locking Plates 1.0 Titanium

**1.0 Locking-Y-Plate Titanium**

3.5 mm / 7.35 mm wide, 1.0 mm thick



Product Code	Description
142-0210-809	10-Hole, 44 mm long

**1.0 MAYO DFO Locking Plate Titanium**

3.5 mm wide, 1.0 mm thick, 9-Hole



Product Code	Description
142-0210-925L	46 mm, cuttable, left 25°
142-0210-925R	46 mm, cuttable, right 25°
142-0210-950L	47.5 mm, cuttable, left 50°
142-0210-950R	47.5 mm, cuttable, right 50°

**1.0 Acetabulum-Locking Plate Titanium**

1.0 mm thick, 4 hole

142-0210-475



**1.0 H-Locking Plate Titanium**

6.3 mm wide, 1.0 mm thick, 10 mm long, 4 hole

142-0210-4H



**LeiLOX Instruments**  
See LeiLOX Instruments on  
Page 112.

**1.0 LeiLOX Locking Screw Titanium**

For LeiLOX Locking System, LeiStar T5 self-holding (T5 Shaft from Rita Leibinger recommended) self-tapping with three flute cutting edge



Length (mm)	Product Code
4	245-410-04
5	245-410-05
6	245-410-06
7	245-410-07
8	245-410-08
9	245-410-09
10	245-410-10
11	245-410-11
12	245-410-12
14	245-410-14
16	245-410-16

**1.3 LeiLOX Locking Screw Titanium**

For LeiLOX Locking System, LeiStar T5 self-holding (T5 Shaft from Rita Leibinger recommended) self-tapping with three flute cutting edge



Length (mm)	Product Code
4	245-413-04
5	245-413-05
6	245-413-06
7	245-413-07
8	245-413-08
9	245-413-09
10	245-413-10
11	245-413-11
12	245-413-12
14	245-413-14
16	245-413-16
18	245-413-18
20	245-413-20


# LeiLOX 1.5/2.0 Micro



## Titanium Locking Fracture System for cats and small dogs

Accidents happen. And you, as a surgeon, are often required to fix complex fractures.

Our 1.5/2.0 locking plate system features 62 different plates, making it the most flexible titanium locking system for small animals. The system can handle both simple and complex fractures.

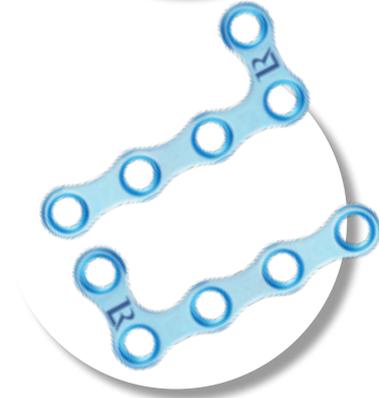

## Titanium: Best Biocompatibility

Unique Titanium Alloy makes our implants very strong, resistant and lightweight, which is ideal for small animals. Titanium offers advantages in biocompatibility, extreme temperatures and weight.



## All-in-One Set

LeiLOX 1.5/2.0 is the "swiss army knife" for micro fractures: it contains not only (cuttable) standard plates, but also unique shapes for complex anatomy, in a compact instrument set.



## Various Applications

With more than 62 different plates, LeiLOX 1.5/2.0 is the perfect solution to treat a wide variety of fracture cases:

Y-Plates, L-Plates, Bridge-Plates, Standard-Plates, Cuttable 20-hole Plates and many Challenger Plates offer plenty of possibilities: from maxillofacial and pelvic fractures, to the fixation of long tubular bones.



## LeiStar Screws

All of our locking screwheads are LeiStar, which allows for best tightening torque.

Additionally, the screws provide a self-holding feature when used with a RITA LEIBINGER screwdriver shaft, keeping the screws securely on the driver.

# LeiLOX

1.5/2.0 MicroLocking System



Special Thanks to  
Dr. Felix Sonntag

## LeiLOX 1.5/2.0 MICRO

**R** RITA  
LEIBINGER  
MEDICAL

## LeiLOX Locking Set 1.5/2.0 Titanium

### 1.5/2.0 Osteosynthesis Locking Set Titanium

Contains:

- 1 Tray for Implants and Instruments with Lid
- 1 Locking Plate of each style (28 pcs. total)
- 5 of each 1.5 Locking Screw (5-24mm, 70 pcs. total)
- 5 of each 2.0 Locking Screw (5-30mm, 85 pcs. total)
- 2 Screwdriver Shafts
- 1 Screwdriver Handle
- 2x2 Locking Drill Guides
- 1 Depth Gauge
- 2 Drills (AO, 1.1 & 1.5)
- 1 pair of Bending Irons

**142-1520-00**

Tray without contents

**142-1520-10**



### 1.5/2.0 Challenger Locking Set Titanium


Contains:

- 1 Implant Tray, without contents
- 1 Locking Plate of each style „Challenger“ (24 pcs. total)

**142-1520-50**

Tray without contents

**142-1520-60**

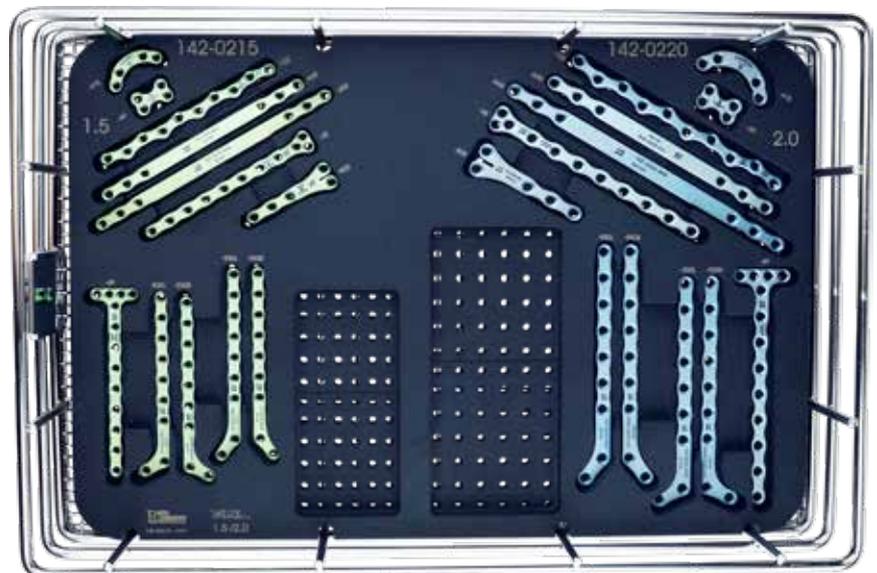

#### **Sterilization Container**

See Sterilization Containers for Implants and Instruments Trays on **Page 204**.

## LeiLOX Locking Set 1.5 Titanium

## LeiLOX Locking Set 2.0 Titanium

### 1.5 Osteosynthesis Locking Set Titanium

Contains:

- 1 Tray for implants and instruments, with lid
- 1 Locking Plate of each style 1.5 mm (26 pcs. total)
- 5 of each 1.5 Locking Screw (5-24mm, 70 pcs. total)
- 1 LeiStar Screwdriver Shaft
- 1 Screwdriver Handle
- 2 Locking Drill Guides
- 1 Depth Gauge
- 1 Drill (AO, 1.1)
- 1 pair of bending irons

**142-1500-00**

Tray without contents

**142-1500-10**



### 2.0 Osteosynthesis Locking Set Titanium

Contains:

- 1 Tray for implants and instruments, with lid
- 1 Locking Plate of each style 2.0mm (26 pcs. total)
- 5 of each 2.0 Locking Screw (5-30mm, 85 pcs. total)
- 1 LeiStar Screwdriver Shaft
- 1 Screwdriver Handle
- 2 Locking Drill Guides
- 1 Depth Gauge
- 1 Drill (AO, 1.5)
- 1 pair of bending irons

**142-2000-00**

Tray without contents

**142-2000-10**



**1520.leibinger.vet**

## LeiLOX Locking Plates 1.5 Titanium

### 1.5 Locking Plate Titanium

5mm wide, 1.5mm thick



Product Code	Description
142-0215-04	4-Hole, 25.5mm
142-0215-05	5-Hole, 32.5mm
142-0215-06	6-Hole, 39.5mm
142-0215-07	7-Hole, 46.5mm
142-0215-08	8-Hole, 53.5mm
142-0215-09	9-Hole, 60.5mm
142-0215-10	10-Hole, 67.5mm
142-0215-20	20-Hole, cuttable

### 1.5 Locking Plate with Bridge, Titanium

5mm wide, 1.5mm thick



Product Code	Description
142-0215-614	14mm Bridge, 4-Hole, 32.5mm
142-0215-621	21mm Bridge, 6-Hole, 53.5mm
142-0215-635	35mm Bridge, 6-Hole, 67.5mm
142-0215-645	45mm Bridge, 6-Hole, 78 mm
142-0215-658	58mm Bridge, 6-Hole, 95mm

### 1.5 T-Locking Plate Titanium

5mm wide, 1.5mm thick, cuttable



Product Code	Description
142-0215-38	1.5 mm, 3/8 hole
142-0215-49	1.5 mm, 4/9 hole

### 1.5 Locking-L-Plate Titanium

5mm / 11.5mm wide, 1.5mm thick, 25.5mm long



Product Code	Description
142-0215-504L	left
142-0215-504R	right

### 1.5 Locking-Y-Plate Titanium


5mm / 11mm wide, 1.5mm thick



Product Code	Description
142-0215-805	5-Hole, 33mm long
142-0215-809	10-Hole, cuttable

### 1.5 MAYO DFO Locking Plate Titanium

5mm wide, 1.5mm thick, 9-Hole

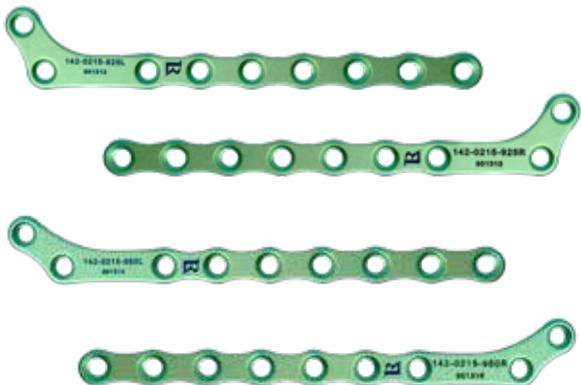

Product Code	Description
142-0215-925L	cuttable, left 25°
142-0215-925R	cuttable, right 25°
142-0215-950L	cuttable, left 50°
142-0215-950R	cuttable, right 50°

## LeiLOX Locking Screws 1.5 Titanium

### 1.5 Z-Locking Plate Titanium

6mm wide, 1.5 mm thick, 10 hole, cuttable  
**142-0215-10Z**



### 1.5 Acetabulum-Locking Plate Titanium

1.5 mm thick, 4 hole  
**142-0215-475**



### 1.5 H-Locking Plate Titanium

9mm wide, 1.5 mm thick, 14mm long, 4 hole  
**142-0215-4H**



### 1.5 LeiLOX Locking Screw Titanium

For LeiLOX Locking System, LeiStar T6  
self-holding (T6 Shaft from Rita Leibinger recommended)  
self-tapping with three flute cutting edge



Length (mm)	Product Code
5	245-415-05
6	245-415-06
7	245-415-07
8	245-415-08
9	245-415-09
10	245-415-10
11	245-415-11
12	245-415-12
14	245-415-14
16	245-415-16
18	245-415-18
20	245-415-20
22	245-415-22
24	245-415-24
26	245-415-26

See more screw lengths on **Page 126.**

Screw Racks on **Page 198.**



### LeiLOX Instruments

See LeiLOX Instruments on  
**Page 112.**



**1520.leibinger.vet**

## LeiLOX Locking Plates 2.0 Titanium

### 2.0 Locking Plate Titanium

6mm wide, 1.5mm thick



Product Code	Description
142-0220-04	4-Hole, 33mm
142-0220-05	5-Hole, 42mm
142-0220-06	6-Hole, 51mm
142-0220-07	7-Hole, 60mm
142-0220-08	8-Hole, 69mm
142-0220-09	9-Hole, 78mm
142-0220-10	10-Hole, 87mm
142-0220-20	20-Hole, cuttable

### 2.0 Locking Plate with Bridge, Titanium


6mm wide, 1.5mm thick



Product Code	Description
142-0220-618	18mm Bridge, 4-Hole, 42mm
142-0220-627	27mm Bridge, 6-Hole, 69mm
142-0220-636	36mm Bridge, 6-Hole, 78mm
142-0220-648	48mm Bridge, 6-Hole, 90mm
142-0220-668	68mm Bridge, 6-Hole, 110mm

### 2.0 T-Locking Plate Titanium

6mm wide, 1.5mm thick, cuttable

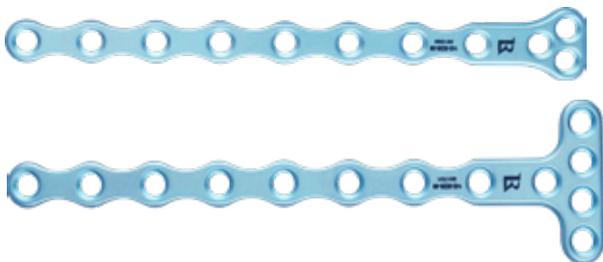

Product Code	Description
142-0220-38	2.0 mm, 3/8 Holes
142-0220-49	2.0 mm, 4/9 Holes

### 2.0 Locking-L-Plate Titanium


6mm / 15mm wide, 1.5mm thick, 33mm long



Product Code	Description
142-0220-504L	left
142-0220-504R	right

### 2.0 Locking-Y-Plate Titanium

6mm / 13.5mm wide, 1.5mm thick

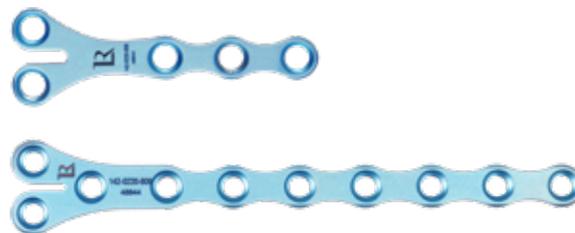

Product Code	Description
142-0220-805	5-Hole, 42mm long
142-0220-809	10-Hole, cuttable

### 2.0 MAYO DFO Locking Plate Titanium

6mm wide, 1.5mm thick, 9-Hole



Product Code	Description
142-0220-925L	cuttable, left 25°
142-0220-925R	cuttable, right 25°
142-0220-950L	cuttable, left 50°
142-0220-950R	cuttable, right 50°

### 2.0 Z-Locking Plate Titanium

8mm wide, 1.5mm thick, 10 Loch, cuttable  
**142-0220-10Z**



### 2.0 Acetabulum-Locking Plate Titanium

1.5mm thick, 4 holes  
**142-0220-410**



### 2.0 H-Locking Plate Titanium

10.5mm wide, 1.5mm thick, 16mm long, 4 holes  
**142-0220-4H**



**LeiLOX Instruments**  
See LeiLOX Instruments on  
**Page 112.**

### 2.0 LeiLOX Locking Screw Titanium

For LeiLOX Locking System, LeiStar T8  
self-holding (T8 Shaft from Rita Leibinger recommended)  
self-tapping with three flute cutting edge



Length (mm)	Product Code
5	245-420-05
6	245-420-06
7	245-420-07
8	245-420-08
9	245-420-09
10	245-420-10
11	245-420-11
12	245-420-12
14	245-420-14
16	245-420-16
18	245-420-18
20	245-420-20
22	245-420-22
24	245-420-24
26	245-420-26
28	245-420-28
30	245-420-30

See more screw lengths on **Page 126.**

Screw Racks on **Page 198.**



## Arthrodesis Plates, LeiLOX Locking, 1.5/2.0 Titanium

### 1.5/2.0 Arthrodesis Plates

locking, bendable, Titanium, 1.5mm thick



LeiLOX Arthrodesis Plate, 1.5/2.0mm,  
55mm long

**142-0215-55**



LeiLOX Arthrodesis Plate, 1.5/2.0mm,  
60mm long

**142-0215-60**



LeiLOX Arthrodesis Plate, 2.0mm,  
60mm long

**142-0220-60**



LeiLOX Arthrodesis Plate, 2.0mm,  
68mm long

**142-0220-68**

### 1.5/2.0 Arthrodesis Plates, angled

locking, bendable, Titanium, 1.5mm thick



LeiLOX Arthrodesis Plate, 1.5/2.0mm,  
56mm long, left

**142-0215-120L**



LeiLOX Arthrodesis Plate, 1.5/2.0mm,  
56mm long, right

**142-0215-120R**



LeiLOX Arthrodesis Plate, 1.5/2.0mm,  
72mm long, left

**142-0215-135L**



LeiLOX Arthrodesis Plate, 1.5/2.0mm,  
72mm long, right

**142-0215-135R**



LeiLOX 2.0 mm  
Dr. Hugo Schmökel



Jaw Surgery / Kieferchirurgie (LeiLOX 1.5 mm)  
Dr. Ilya Zhuravchak



# LeiLOX 2.0/2.4 & 2.7/3.5 Locking System



## Multiaxial Locking

The screws can be locked in 90° angle with a 12° deviation in any direction. This allows you to angle specific screws away from vital structures. The robust LeiStar screw head locks firmly into the plate.



## Straight, Bridge, Reconstruction & Arthrodesis Plates

LeiLOX offers you the right plate for every fracture. It offers not only Straight, but also Bridge, Reconstruction and Arthrodesis Plates.

Further you get bending irons that comfortably bend the plates in any direction.

Locking Plugs offer additional strength and protect the screw holes when you bend the plates.



## Straight Plates


Straight plates are needed in strong bones that face high forces. With our bending irons, they can be bent vertically.

Straight plates feature limited contact dynamic compression to minimize vascular damage to the plated bone segment.



## Interchangeable 2.0/2.4 & 2.7/3.5mm Screws

Because the screw heads are identical, all Stainless Steel 2.0/2.4 respectively 2.7/3.5 LeiLOX plates (TPLO and fracture systems) work with 2.0mm as well as 2.4mm screws respectively 2.7mm as well as 3.5mm screws in all plate sizes. This offers flexibility and saves on inventory cost.

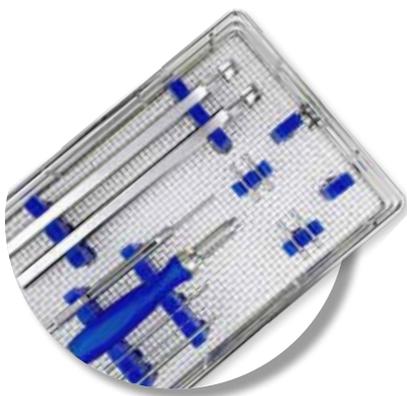


## Universal Instrumentation

Locking drill guides, screw drivers, depth gauge, etc. are identical and interchangeable in all of our 2.0/2.4 respectively 2.7/3.5 systems (Fracture Systems as well as TPLO and CBLO).

SIN

# LeiLOX

2.0-3.5 Locking System

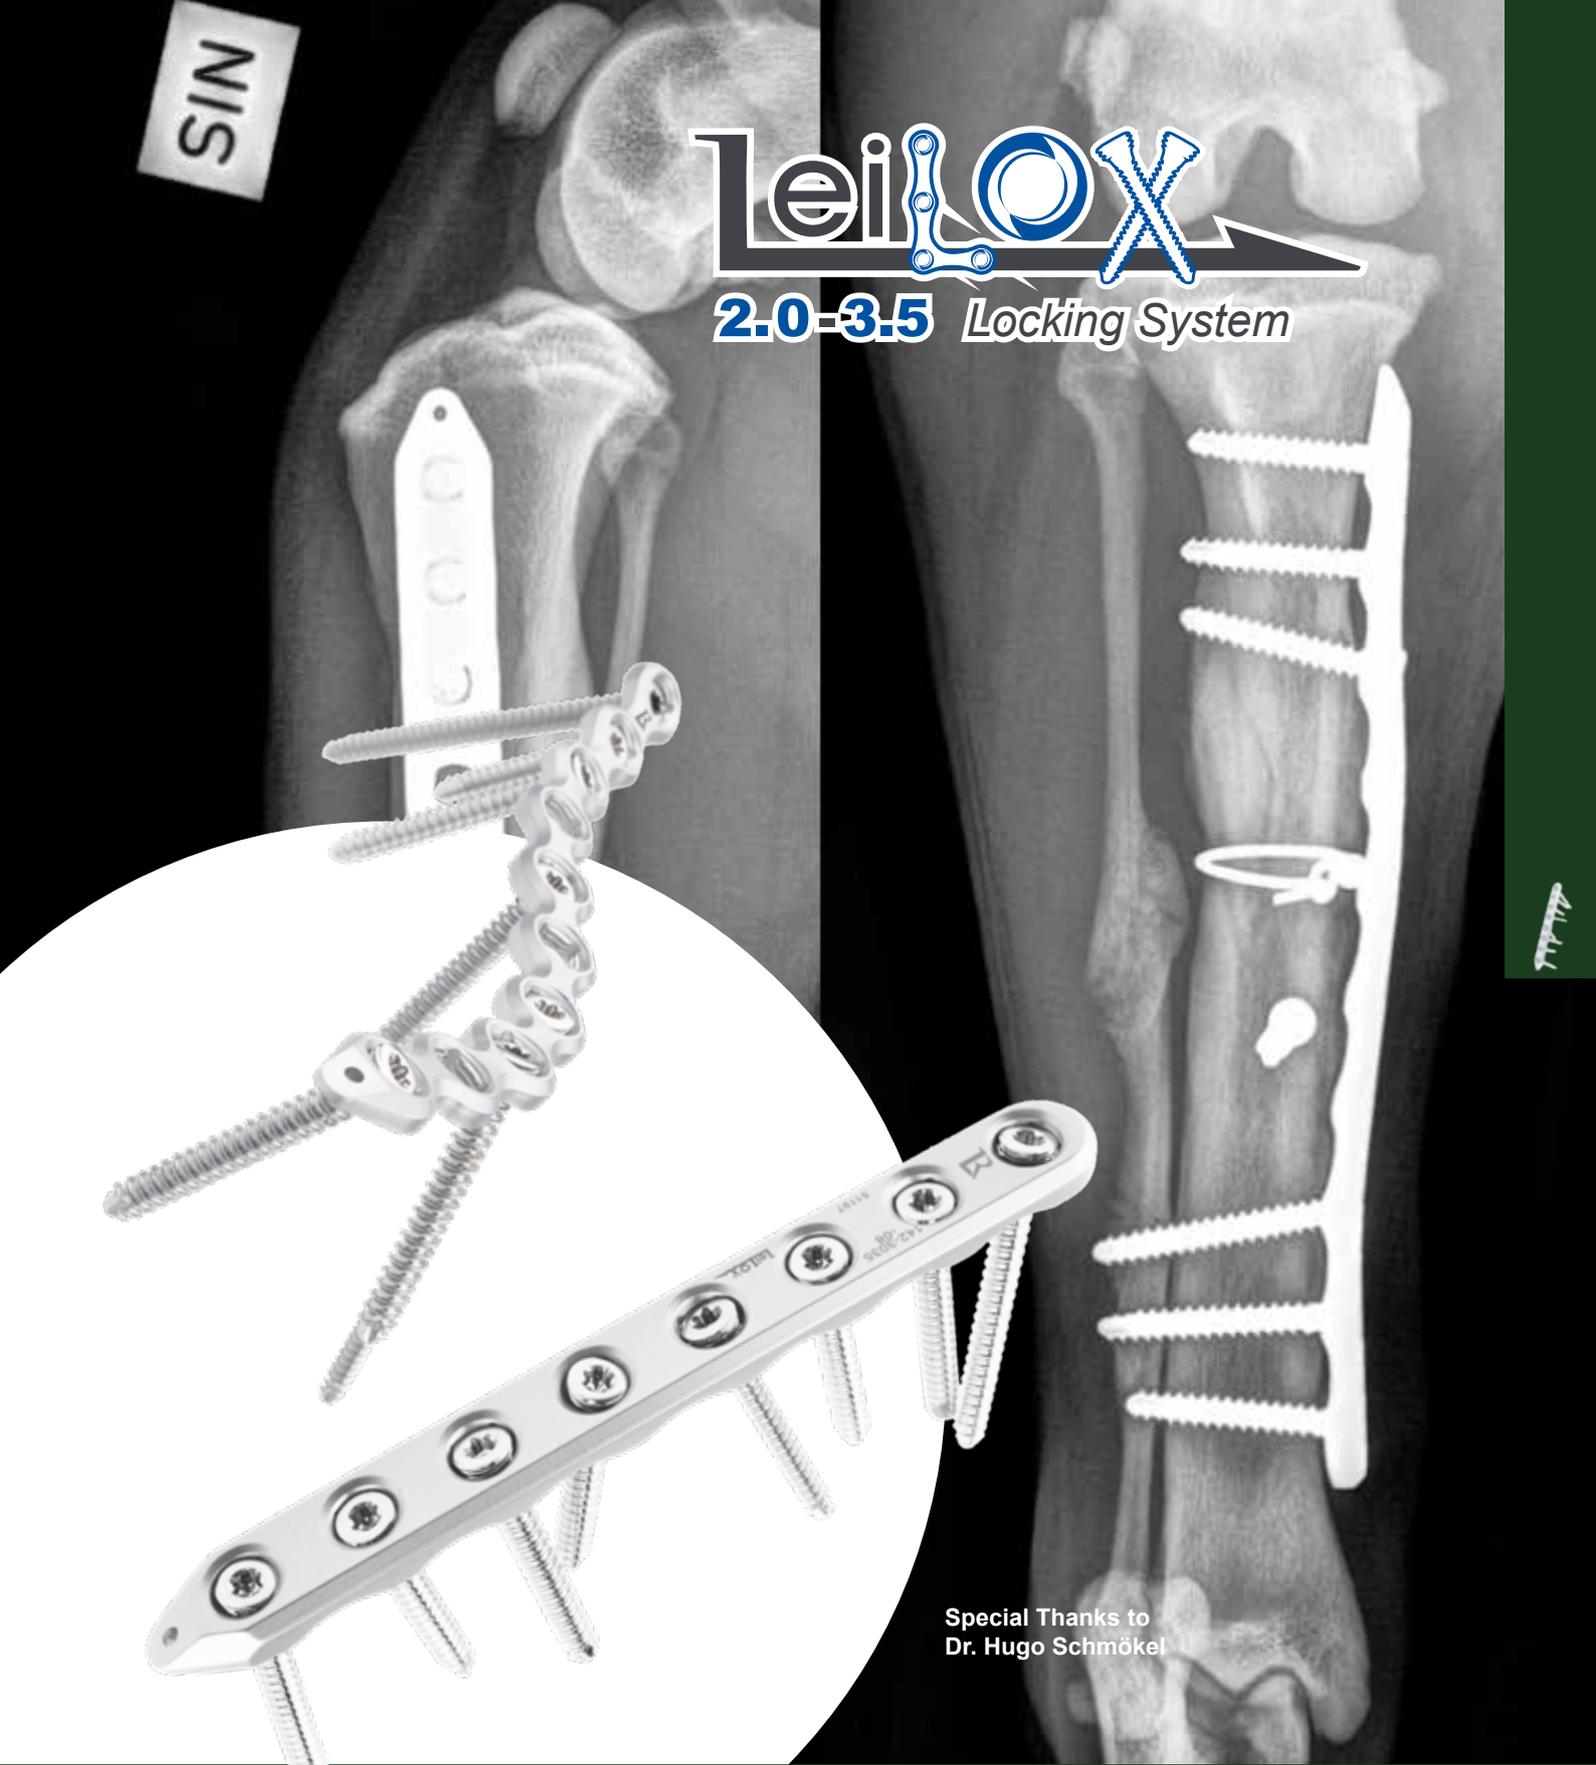

Special Thanks to  
Dr. Hugo Schmökel

## LeiLOX 2.0/3.5

## LeiLOX Sets, Straight Plates 2.0/2.4 + 2.7/3.5


### 2.0/2.4 Straight Implant Set

Contains:

- 1 Tray for Implants with Lid, stackable
- 1 of each Plate  
(24 pcs. total)
- 5 of each 2.0 Locking Screw  
(6-30mm, 65 pcs. total)
- 5 of each 2.4 Locking Screw  
(6-40mm, 90 pcs. total)

Complete Set  
**142-2024-00**

Tray without contents  
**142-2024-01**

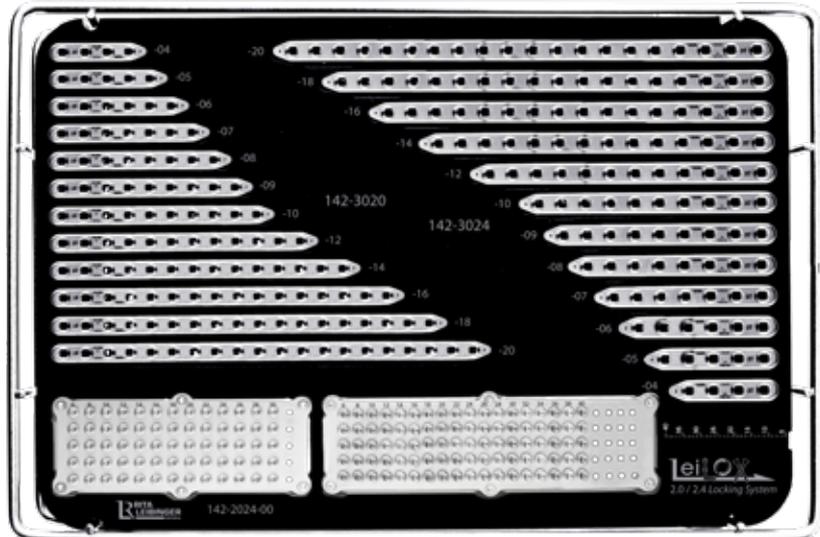


### 2.7/3.5 Straight Implant Set

Contains:

- 1 Tray for Implants with Lid, stackable
- 1 Screwrack 2.7
- 1 Screwrack 3.5
- 1 of each Plate  
(24 pcs. total)
- 5 of each 2.7 Locking Screw  
(10-46mm, 95 pcs. total)
- 5 of each 3.5 Locking Screw  
(10-50mm, 100 pcs. total)

Complete Set  
**142-3000-00**

Tray without contents  
**142-3010-02**

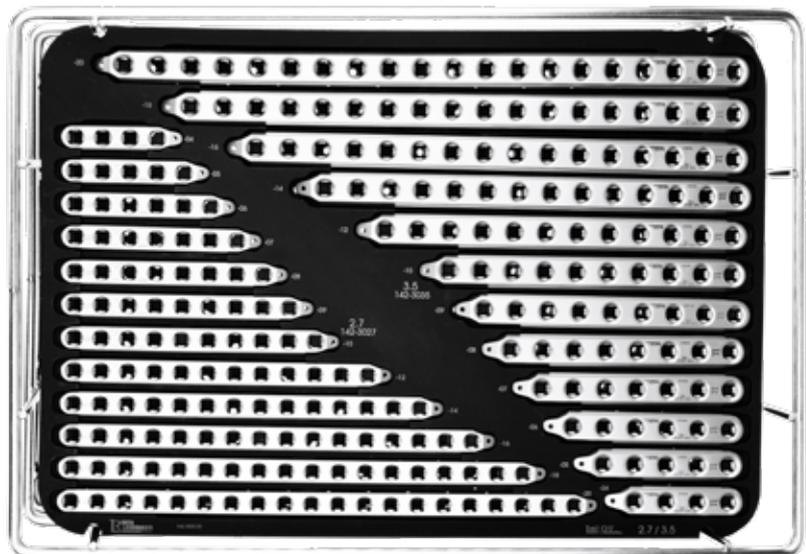

LeiLOX Sets, Straight Plates 2.0/2.4 + 2.7/3.5

LeiLOX Set, Arthrodesis 2.0-3.5


**2.0/2.4 Bridge Plate Set**

Contains:  
1 Tray for Implants with Lid, stackable  
1 of each Plate  
(20 pcs. total)

Complete Set (without screws)  
**142-2024-60**

Tray without contents  
**142-2024-62**

See Screws (optional) on **Page 108.**

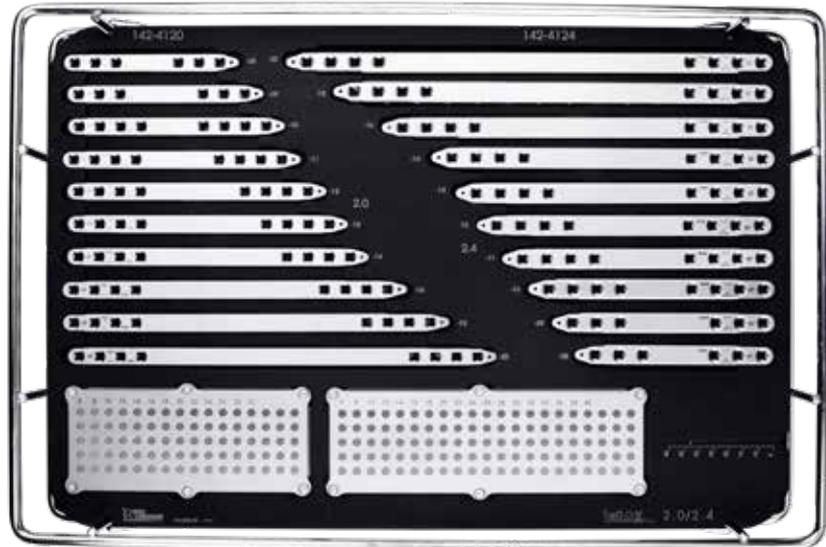

**2.7/3.5 Bridge Plate Set**


Contains:  
1 Tray for Implants with Lid, stackable  
1 of each Bridge Plate  
(20 pcs. total)

Complete Set (without Screws)  
**142-3200-00**

Tray without contents  
**142-3200-10**

See Screws (optional) on **Page 108.**

See Screw Racks (optional) on **Page 198.**

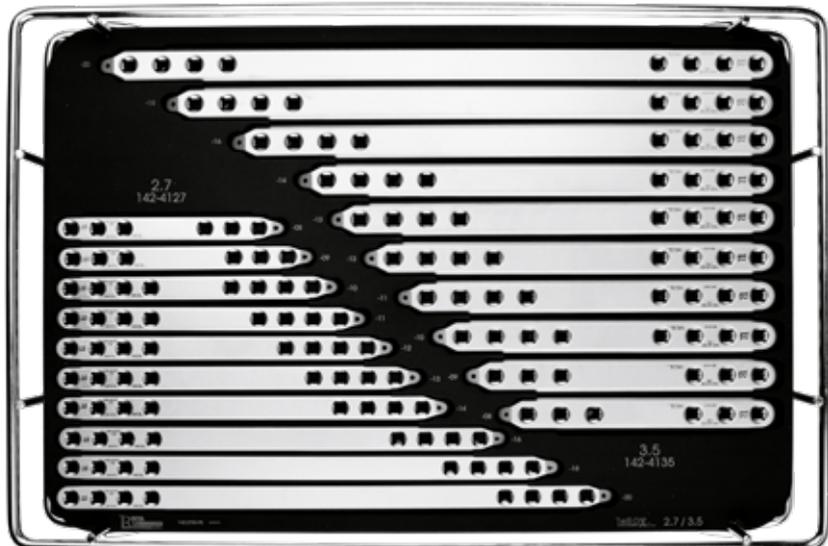

**2.0-3.5 Arthrodesis Set**


Contains:  
1 Tray for Implants with Lid, stackable  
1 of each Arthrodesis Plate  
(16 pcs. total)

Complete Set (without Screws)  
**142-3300-00**

Tray without contents  
**142-3300-10**

See Screws (optional) on **Page 108.**

See Screw Racks (optional) on **Page 198.**

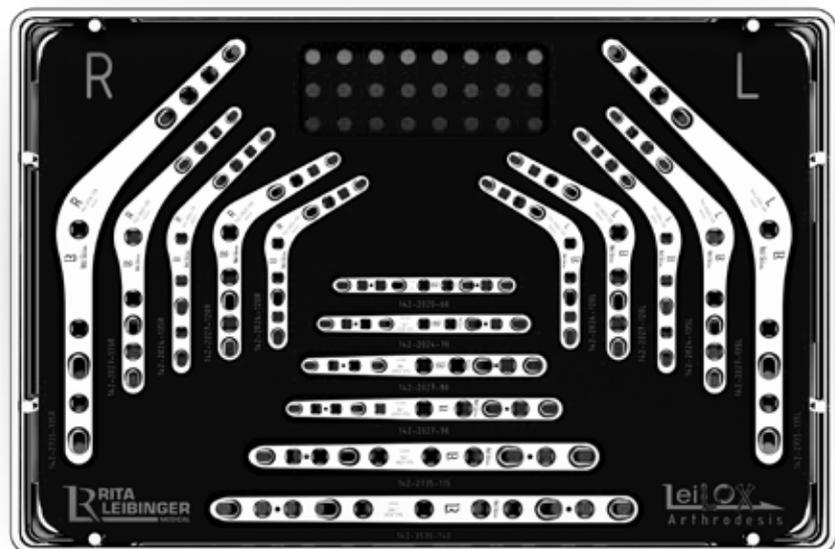

LeiLOX Sets, Reconstruction 2.0/2.4 + 2.7/3.5

**2.0/2.4 Reconstruction Implant Set**


Contains:

- 1 Tray for Implants with Lid
- 1 of each Plate  
(24 pcs. total)
- 5 of each 2.0 Locking Screw  
(06-30mm, 65 pcs. total)
- 5 of each 3.4 Locking Screw  
(6-40mm, 90 pcs. total)

**142-2024-90**

Tray without contents

**142-2024-91**

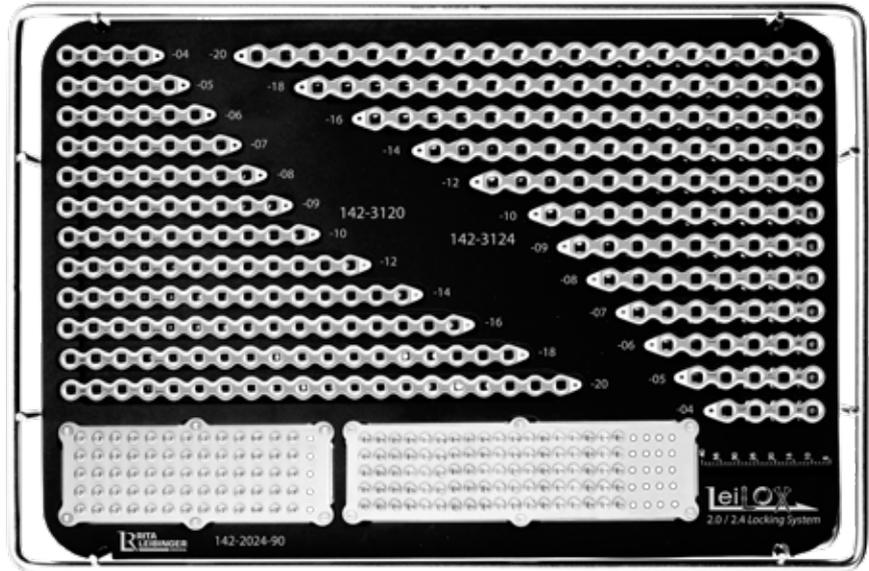

**2.7/3.5 Reconstruction Implant Set**




Contains:

- Tray for Reconstruction Implants with Lid
- 1 Screwrack 2.7
- 1 Screwrack 3.5
- 1 of each Plate (24 pcs. total)
- 5 of each 2.7 Locking Screw  
(10-46mm, 95 pcs. total)
- 5 of each 3.5 Locking Screw  
(12-50mm, 100 pcs. total)

**142-3100-00**

Tray without contents

**142-3100-02**

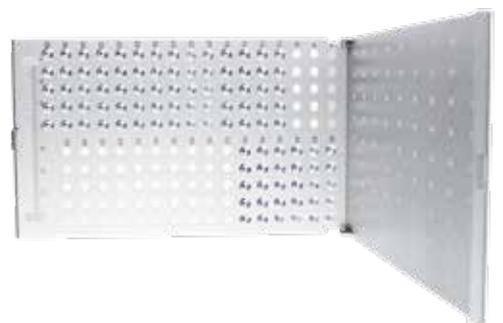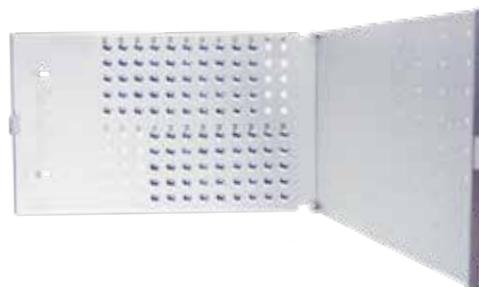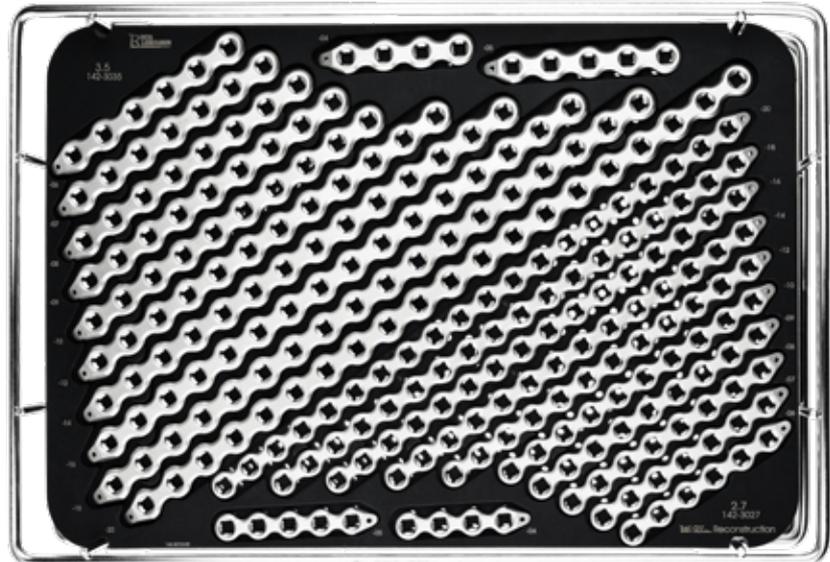

**LeiLOX Sets, Straight + Reconstruction 2.0/2.0 + 2.4/2.4 + 2.7/2.7**


**2.0/2.0 Straight + Reconstruction Implant Set**

- Contains:
- Tray for Implants with Lid
- 1 of each Plate  
(24 pcs. total)
- 5 of each 2.0 Locking Screw  
(6-30mm, 65 pcs. total)

**142-2020-00**

Tray without contents

**142-2020-01**

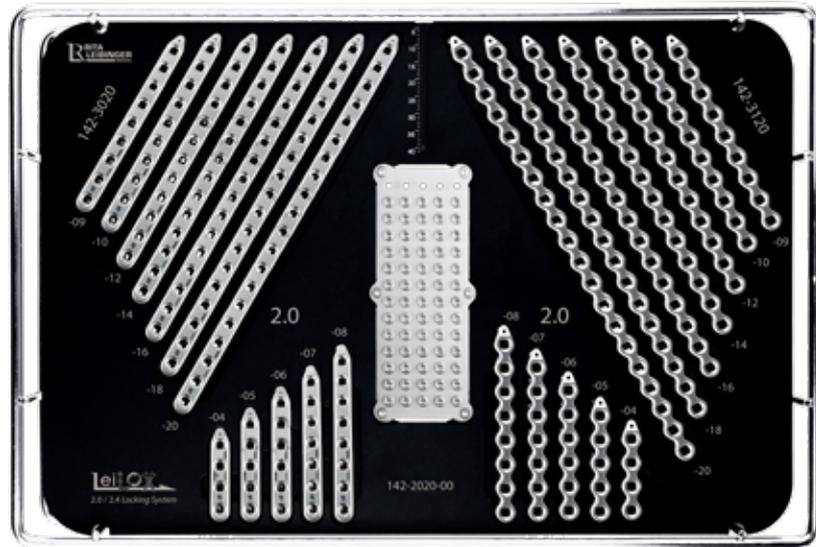


**2.4/2.4 Straight + Reconstruction Implant Set**

- Contains:
- Tray for Implants with Lid
- 1 of each Plate  
(24 pcs. total)
- 5 of each 2.0 Locking Screw  
(6-40mm, 90 pcs. total)

**142-2424-00**

Tray without contents

**142-2424-01**

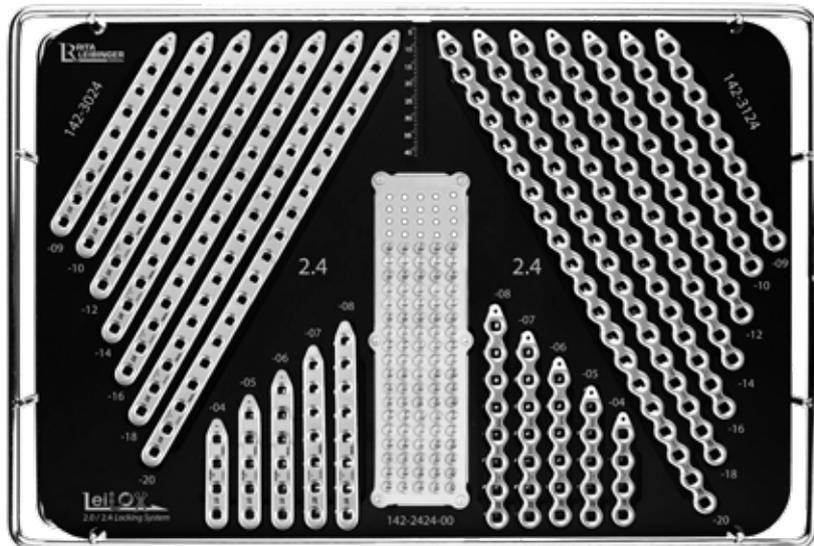


**2.7/2.7 Straight + Reconstruction Implant Set**

- Contains:
- Tray for Implants with Lid
- 1 of each Bone Plate  
(12 pcs. total)
- 1 of each Reconstruction Plate  
(12 pcs. total)
- 1 Screw rack 2.7
- 5 of each 2.7 Locking Screw  
(10-50mm, 105 pcs. total)

**142-2727-00**

Tray without contents

**142-2727-01**

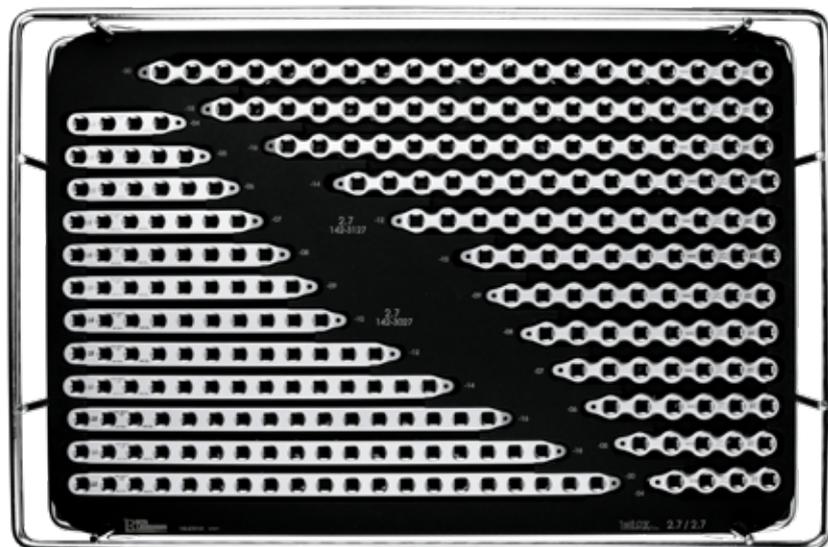

## Straight Plate, LeiLOX Locking, Stainless Steel

### 2.0 LeiLOX Boneplate

Multiaxial locking, straight, Stainless Steel  
compatible with 2.0 & 2.4mm LeiLOX Screws

 1.7 mm thick  6 mm wide



Product Code	Holes	Length (mm)
142-3020-04	4	31.5
142-3020-05	5	38.5
142-3020-06	6	45.5
142-3020-07	7	52.5
142-3020-08	8	59.5
142-3020-09	9	66.5
142-3020-10	10	73.5
142-3020-12	12	87.5
142-3020-14	14	101.5
142-3020-16	16	115.5
142-3020-18	18	129.5
142-3020-20	20	143.5

### 2.4 LeiLOX Boneplate

multiaxial locking, straight, Stainless Steel  
compatible with 2.0 & 2.4mm LeiLOX Screws

 2.3 mm thick  7 mm wide



Product Code	Holes	Length (mm)
142-3024-04	4	35.5
142-3024-05	5	43.5
142-3024-06	6	51.5
142-3024-07	7	59.5
142-3024-08	8	67.5
142-3024-09	9	75.5
142-3024-10	10	83.5
142-3024-12	12	99.5
142-3024-14	14	115.5
142-3024-16	16	131.5
142-3024-18	18	147.5
142-3024-20	20	163.5

### 2.7 LeiLOX Boneplate

Multiaxial locking, straight, Stainless Steel  
compatible with 2.7 & 3.5mm LeiLOX Screws

 3 mm thick  9 mm wide



Product Code	Holes	Length (mm)
142-3027-04	4	40
142-3027-05	5	49
142-3027-06	6	58
142-3027-07	7	67
142-3027-08	8	76
142-3027-09	9	85
142-3027-10	10	94
142-3027-12	12	112
142-3027-14	14	130
142-3027-16	16	148
142-3027-18	18	166
142-3027-20	20	184

### 3.5 LeiLOX Boneplate

Multiaxial locking, straight, Stainless Steel  
compatible with 2.7 & 3.5mm LeiLOX Screws

 4 mm thick  11 mm wide



Product Code	Holes	Length (mm)
142-3035-04	4	49
142-3035-05	5	60
142-3035-06	6	71
142-3035-07	7	82
142-3035-08	8	93
142-3035-09	9	104
142-3035-10	10	115
142-3035-12	12	137
142-3035-14	14	159
142-3035-16	16	181
142-3035-18	18	203
142-3035-20	20	225

## Bridge Plate, LeiLOX Locking, Stainless Steel

### 2.0 LeiLOX Bridge Plate

Multiaxial locking, straight, Stainless Steel  
compatible with 2.0 & 2.4mm LeiLOX Screws

 1.7 mm thick  6 mm wide



Product Code	Holes	Length (mm)	
		Total	Bridge
142-4120-08	6	59.5	17
142-4120-09	6	66.5	24
142-4120-10	8	73.5	17
142-4120-11	8	80.5	24
142-4120-12	8	87.5	31
142-4120-13	8	94.5	38
142-4120-14	8	101.5	45
142-4120-16	8	115.5	59
142-4120-18	8	129.5	73
142-4120-20	8	143.5	87

### 2.4 LeiLOX Bridge Plate

Multiaxial locking, straight, Stainless Steel  
compatible with 2.0 & 2.4mm LeiLOX Screws

 2.3 mm thick  7 mm wide



Product Code	Holes	Length (mm)	
		Total	Bridge
142-4124-08	6	67.5	20
142-4124-09	6	75.5	28
142-4124-10	8	83.5	20
142-4124-11	8	91.5	28
142-4124-12	8	99.5	36
142-4124-13	8	107.5	44
142-4124-14	8	115.5	52
142-4124-16	8	131.5	68
142-4124-18	8	147.5	84
142-4124-20	8	163.5	100

### 2.7 LeiLOX Bridge Plate

Multiaxial locking, straight, Stainless Steel  
compatible with 2.7 & 3.5mm LeiLOX Screws

 3 mm thick  9 mm wide



Product Code	Holes	Length (mm)	
		Total	Bridge
142-4127-08	6	76	22
142-4127-09	6	85	31
142-4127-10	8	94	22
142-4127-11	8	103	31
142-4127-12	8	112	40
142-4127-13	8	121	48
142-4127-14	8	130	57
142-4127-16	8	148	75
142-4127-18	8	166	93
142-4127-20	8	184	111

### 3.5 LeiLOX Bridge Plate

Multiaxial locking, straight, Stainless Steel  
compatible with 2.7 & 3.5mm LeiLOX Screws

 4 mm thick  11 mm wide



Product Code	Holes	Length (mm)	
		Total	Bridge
142-4135-08	6	93	27
142-4135-09	6	104	38
142-4135-10	8	115	27
142-4135-11	8	126	38
142-4135-12	8	137	49
142-4135-13	8	148	60
142-4135-14	8	159	71
142-4135-16	8	181	93
142-4135-18	8	203	115
142-4135-20	8	225	137

## Reconstruction Plate, LeiLOX Locking, Stainless Steel

### 2.0 LeiLOX Reconstruction Plate

Multiaxial locking, bendable, Stainless Steel compatible with 2.0 & 2.4mm LeiLOX Screws

 1.7 mm thick  6.5 mm wide



Product Code	Holes	Length (mm)
142-3120-04	4	34
142-3120-05	5	42
142-3120-06	6	50
142-3120-07	7	58
142-3120-08	8	66
142-3120-09	9	74
142-3120-10	10	82
142-3120-12	12	98
142-3120-14	14	114
142-3120-16	16	130
142-3120-18	18	146
142-3120-20	20	162

### 2.4 LeiLOX Reconstruction Plate

Multiaxial locking, bendable, Stainless Steel compatible with 2.0 & 2.4mm LeiLOX Screws

 2.3 mm thick  7 mm wide



Product Code	Holes	Length (mm)
142-3124-04	4	37.5
142-3124-05	5	46.5
142-3124-06	6	55.5
142-3124-07	7	64.5
142-3124-08	8	73.5
142-3124-09	9	82.5
142-3124-10	10	91.5
142-3124-12	12	109.5
142-3124-14	14	127.5
142-3124-16	16	145.5
142-3124-18	18	163.5
142-3124-20	20	181.5

### 2.7 LeiLOX Reconstruction Plate

Multiaxial locking, bendable, Stainless Steel compatible with 2.7 & 3.5mm LeiLOX Screws

 3 mm thick  9 mm wide



Product Code	Holes	Length (mm)
142-3127-04	4	40
142-3127-05	5	49
142-3127-06	6	58
142-3127-07	7	67
142-3127-08	8	76
142-3127-09	9	85
142-3127-10	10	94
142-3127-12	12	112
142-3127-14	14	130
142-3127-16	16	148
142-3127-18	18	166
142-3127-20	20	184

### 3.5 LeiLOX Reconstruction Plate

Multiaxial locking, bendable, Stainless Steel compatible with 2.7 & 3.5mm LeiLOX Screws

 4 mm thick  11 mm wide



Product Code	Holes	Length (mm)
142-3135-04	4	49
142-3135-05	5	60
142-3135-06	6	71
142-3135-07	7	82
142-3135-08	8	93
142-3135-09	9	104
142-3135-10	10	115
142-3135-12	12	137
142-3135-14	14	159
142-3135-16	16	181
142-3135-18	18	203
142-3135-20	20	225

T-Plate, LeiLOX Locking, Stainless Steel

**NEW**

**2.0 LeiLOX T-Plate**

Multiaxial locking, Stainless Steel  
compatible with 2.0 & 2.4mm LeiLOX Screws



Product Code	Holes	Size (in mm)		
		L	W	W1
142-3620-35	3 x 4	49.5	11	6
142-3620-37	3 x 5	63.5	11	6

**2.4 LeiLOX T-Plate**


Multiaxial locking, Stainless Steel  
compatible with 2.0 & 2.4mm LeiLOX Screws



Product Code	Holes	Size (in mm)		
		L	W	W1
142-3624-35	3 x 4	57.5	13	7
142-3624-37	3 x 5	73.5	13	7

**2.7 LeiLOX T-Plate**


Multiaxial locking, Stainless Steel  
compatible with 2.7 & 3.5mm LeiLOX Screws

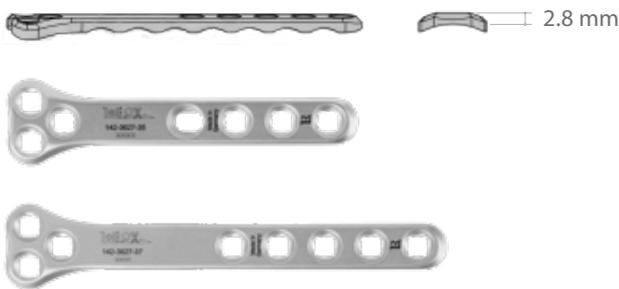

Product Code	Holes	Size (in mm)		
		L	W	W1
142-3627-35	3 x 4	68.5	17	9
142-3627-37	3 x 5	86.5	17	9

**3.5 LeiLOX T-Plate**

Multiaxial locking, Stainless Steel  
compatible with 2.7 & 3.5mm LeiLOX Screws

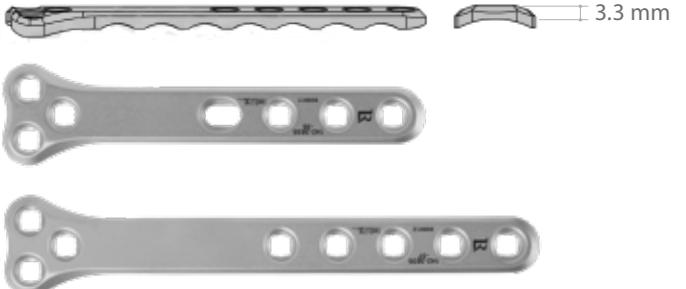

Product Code	Holes	Size (in mm)		
		L	W	W1
142-3635-35	3 x 4	82.5	20	11
142-3635-37	3 x 5	104.5	20	11



**LeiLOX Instruments**  
See LeiLOX Instruments on  
Page 112.



## Arthrodesis Plates, LeiLOX Locking, Stainless Steel

### LeiLOX Arthrodesis Plate, straight

Multiaxial locking, bendable, Stainless Steel  
compatible with 2.0/2.4mm and 2.7/3.5 LeiLOX Screws

#### 2.0 / 2.0 mm

60 mm long

**142-2020-60**



#### 2.4 / 2.0 mm

70 mm long

**142-2024-70**



#### 2.7 / 2.0 mm

80 mm long

**142-2027-80**



#### 2.7 / 2.0 mm

90 mm long

**142-2027-90**



#### 2.7 / 3.5 mm

115 mm long

**142-2735-115**



#### 3.5 / 3.5 mm

140 mm long

**142-3535-140**



## LeiLOX Arthrodesis Plate, angled

Multiaxial locking, bendable, Stainless Steel  
compatible with 2.0/2.4mm and 2.7/3.5 LeiLOX Screws

### 2.0 / 2.4 mm

64 mm long

#### Product Code

<b>142-2024-120L</b>	left
<b>142-2024-120R</b>	right



### 2.0 / 2.7 mm

77 mm long

#### Product Code

<b>142-2027-120L</b>	left
<b>142-2027-120R</b>	right



### 2.0 / 2.4 mm

86 mm long

#### Product Code

<b>142-2024-135L</b>	left
<b>142-2024-135R</b>	right



### 2.0 / 2.7 mm

100 mm long

#### Product Code

<b>142-2027-135L</b>	left
<b>142-2027-135R</b>	right



### 2.7 / 3.5 mm

150 mm long

#### Product Code

<b>142-2735-135L</b>	left
<b>142-2735-135R</b>	right



## Cortical Screws, LeiLOX Locking, Stainless Steel

### LeiLOX Locking Cortical Screws Stainless Steel

For LeiLOX Locking Systems, LeiStar T8 (2.0/2.4) & T10 (2.7/3.5)  
self-holding (Shaft from Rita Leibinger recommended)  
self-tapping with three flute cutting edge



Length (mm)	2.0 mm	2.4 mm	2.7 mm	3.5 mm
	Product Code	Product Code	Product Code	Product Code
6	242-120-06	242-124-06		
8	242-120-08	242-124-08		
10	242-120-10	242-124-10	242-127-10	242-135-10
12	242-120-12	242-124-12	242-127-12	242-135-12
14	242-120-14	242-124-14	242-127-14	242-135-14
16	242-120-16	242-124-16	242-127-16	242-135-16
18	242-120-18	242-124-18	242-127-18	242-135-18
20	242-120-20	242-124-20	242-127-20	242-135-20
22	242-120-22	242-124-22	242-127-22	242-135-22
24	242-120-24	242-124-24	242-127-24	242-135-24
26	242-120-26	242-124-26	242-127-26	242-135-26
28	242-120-28	242-124-28	242-127-28	242-135-28
30	242-120-30	242-124-30	242-127-30	242-135-30
32		242-124-32	242-127-32	242-135-32
34		242-124-34	242-127-34	242-135-34
36		242-124-36	242-127-36	242-135-36
38		242-124-38	242-127-38	242-135-38
40		242-124-40	242-127-40	242-135-40
42			242-127-42	242-135-42
44			242-127-44	242-135-44
46			242-127-46	242-135-46
48			242-127-48	242-135-48
50			242-127-50	242-135-50
52				242-135-52
54				242-135-54
56				242-135-56
58				242-135-58
60				242-135-60
62				242-135-62
64				242-135-64
66				242-135-66
68				242-135-68
70				242-135-70

### Locking Plug for LeiLOX

LeiStar, 1.5mm K-Wire hole, for 2.0/2.4 & 2.7/3.5 plates self-holding (shaft from Rita Leibinger recommended)



Product Code	Description
242-0020-24	2.0 / 2.4 mm
242-0027-35	2.7 / 3.5 mm



top



bottom




side



#### Fixation

Create an additional K-Wire fixation point in any hole of the plate.

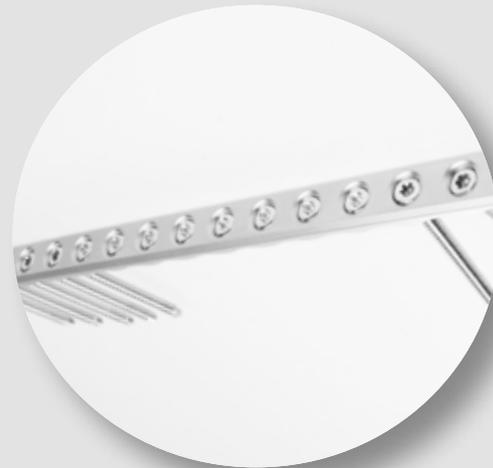

#### Stability

Increase the fatigue strength by closing unused screw holes.



#### Protection

Protect the screw holes while bending the plate.



[2024.leibinger.vet](https://2024.leibinger.vet)



[2735.leibinger.vet](https://2735.leibinger.vet)

## Cortical Screws, Non-Locking, Stainless Steel

### Cortical Screw (Non-Locking) Stainless Steel

LeiStar T8 (2.0/2.4) & T10 (2.7/3.5) self-holding (Shaft from Rita Leibinger recommended) self-tapping with three flute cutting edge




Length (mm)	2.0 mm	2.4 mm	2.7 mm	3.5 mm
	Product Code	Product Code	Product Code	Product Code
8	245-620-08	245-624-08		
10	245-620-10	245-624-10		
12	245-620-12	245-624-12		
14	245-620-14	245-624-14		
16	245-620-16	245-624-16	245-627-16	245-635-16
18	245-620-18	245-624-18	245-627-18	245-635-18
20		245-624-20	245-627-20	245-635-20
22		245-624-22	245-627-22	245-635-22
24		245-624-24	245-627-24	245-635-24
26		245-624-26	245-627-26	245-635-26
28		245-624-28	245-627-28	245-635-28
30		245-624-30	245-627-30	245-635-30
32		245-624-32	245-627-32	245-635-32
34		245-624-34	245-627-34	245-635-34
36		245-624-36	245-627-36	245-635-36
38		245-624-38	245-627-38	245-635-38
40		245-624-40	245-627-40	245-635-40
45				245-635-45
50				245-635-50
55				245-635-55
60				245-635-60

See more screw lengths on **Page 126.**

Screw Racks on **Page 198.**

# LeILOX

**1.0 / 1.3 Nano**  
**1.5 / 2.0 Micro**  
**2.0-3.5 Stainless Steel**

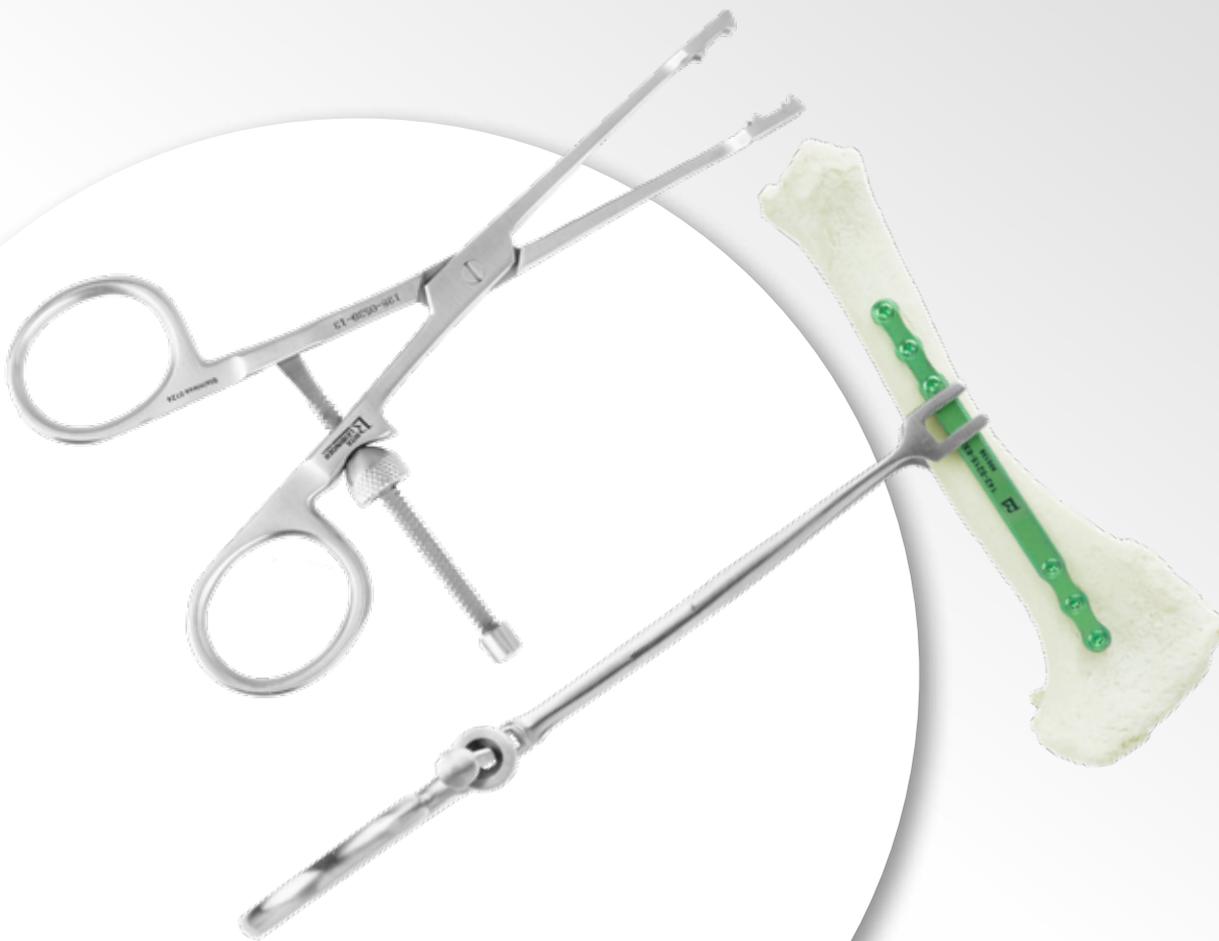

## INSTRUMENTS

**R** RITA  
LEIBINGER  
MEDICAL

**LeiLOX Instrument Set**

2.0-3.5  
Steel

Contains:


- Tray for 2.0/2.4 Instruments
- 2 Drills (1.5 & 1.8mm)
- 2x K-Wires (1.0mm)
- 2x2 Locking Drill Guides
- 1 Screwdriver Handle
- 1 Screwdriver Shaft
- 1 Depth Gauge
- 1 Pair Bending Irons

2.0/2.4 Instruments Set  
**142-2024-50**

2.0/2.4 Tray without contents  
**142-2024-51**

2.7/3.5 Instruments Set  
**142-3010-00**

2.7/3.5 Tray without contents  
**142-3010-01**

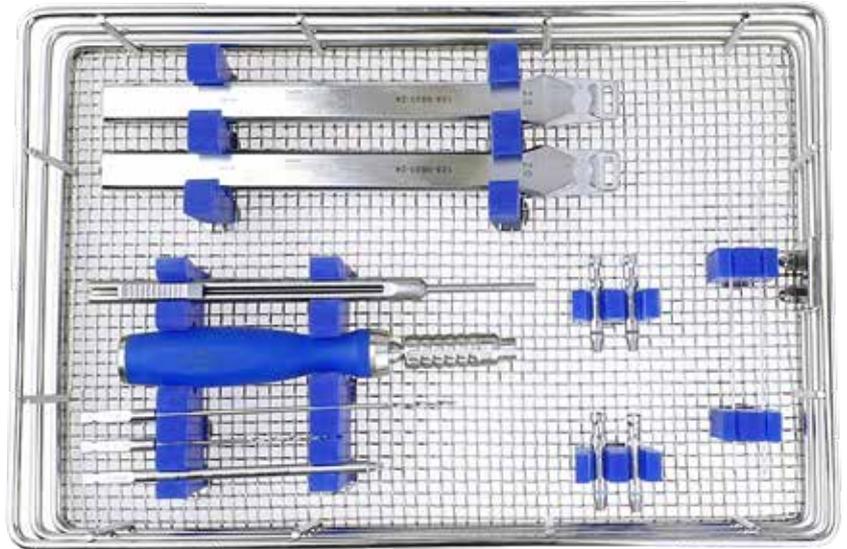

**Sterilization Container**

See Sterilization Containers for Implants and Instruments Trays on **Page 204**.



**Screw Racks**

See screw racks for 1.5mm up to 3.5mm screws on **Page 198**.

**Bending Iron AO Type 1.5/2.0**

130 mm, Pair

1.0 / 1.3  
Nano

1.5 / 2.0  
Micro

**128-0881-15**



**Bending Iron**

2.0-3.5  
Steel



Product Code	Description
<b>128-0820-24</b>	Pair, for 2.0/2.4 Straight & Reconstruction Plates
<b>128-0827-35</b>	Pair, for 2.7/3.5 Straight & Reconstruction Plates

**Bone Plate Holding Forceps**

**Bone Plate Holding Retractor**

**Bone Plate Cutter**

**LEIKUTA Bone Plate Holding Forceps**

140mm, straight with spin lock,  
45 mm working end

1.5 / 2.0  
Micro

**128-0539-13**



**NEW**

Now features a spin lock  
for gentle application



**LEIKUTA Bone Plate Holding Forceps**

135mm, angled up with spin lock,  
45 mm working end

1.5 / 2.0  
Micro

**128-0538-13**



**Bone Plate Holding Retractor**

angled up, with tensioning screw, working end 10x4mm

1.5 / 2.0  
Micro

**128-0537-10**



**Bone Plate Cutter**

Double action, for titanium plates max. 1.5 mm

1.5 / 2.0  
Micro

**23-5865-24T**



## Drills with Round Shaft



1.0 / 1.3  
Nano

1.5 / 2.0  
Micro

2.0-3.5  
Steel

Product Code	Ø (mm)	for Screw Ø (mm)	Length (mm)
148-0080-07	0.7	for 1.0 screws	45
148-0080-10	1.0	for 1.3 screws	45
148-0080-11	1.1	for 1.5 screws	45
148-0180-11	1.1	for 1.5 screws	85
148-0080-15	1.5	for 2.0 screws	70
148-0180-15	1.5	for 2.0 screws	130
148-0080-18	1.8	for 2.4 screws	125
148-0080-20	2.0	for 2.7 screws	85

## Drills with AO Schaft



self-centering



1.0 / 1.3  
Nano

1.5 / 2.0  
Micro

2.0-3.5  
Steel

Product Code	Ø (mm)	for Screw Ø (mm)	Length (mm)
148-0081-07	0.7	for 1.0 screws	72 / 47
148-0081-10	1.0	for 1.3 screws	72 / 47
148-0081-11	1.1	for 1.5 screws	60 / 35
148-0181-11	1.1	for 1.5 screws	85 / 60
148-0081-15	1.5	for 2.0 screws	85 / 60
148-0181-15	1.5	for 2.0 screws	110 / 85
148-0081-18	1.8	for 2.4 screws	125 / 25
148-0081-20	2.0	for 2.7 screws	100 / 75

See more Twist Drills on **Page 199**.

### Locking Drill Guide

1.0 / 1.3  
Nano

Product Code	Description
164-0010-00	for 1.0 mm Screws, 0.7 mm Drill
164-0013-00	for 1.3 mm Screws, 1.0 mm Drill



### Locking Drill Guide

1.5 / 2.0  
Micro

Product Code	Description
164-0015-00	for 1.5 mm Screws, 1.1 mm Drill
164-0020-00	for 2.0 mm Screws, 1.5 mm Drill



### Locking Drill Guide

2.0-3.5  
Steel

Product Code	Description
164-2000-00	for 2.0 mm screws, 1.5 mm Drill
164-2400-00	for 2.4 mm screws, 1.8 mm Drill
164-2700-00	for 2.7 mm screws, 2.0 mm Drill
164-3500-00	for 3.5 mm screws, 2.5 mm Drill



### Depth Gauge

1.0 / 1.3  
Nano

1.5 / 2.0  
Micro

2.0-3.5  
Steel



Product Code	Description	Compatibility
164-1013-20	150mm in length, scale up to 20mm	for 1.0/1.3/1.5 mm screws
164-1520-20	150mm in length, scale up to 40mm	for 1.5/2.0/2.4 mm screws
164-2735-60	150mm in length, scale up to 60mm	for 2.4/2.7/3.5 mm screws

**K-Wire**

Single Trocar  
1.0 mm x 100 mm



Product Code	Dimensions (mm)
144-1010-10	1.0 x 100
144-1020-10	2.0 x 100
144-1025-10	2.5 x 100
144-1030-10	3.0 x 100

See more K-Wires on **Page 136**.

**Screwdriver Shaft LeiStar**

AO connection, self-holding  
(no Holding Sleeve needed)

1.0 / 1.3  
**Nano**

1.5 / 2.0  
**Micro**

2.0-3.5  
**Steel**



Product Code	Description
128-1013-00	T5, for 1.0 mm Screws, 60 mm length
128-1520-15	T6, for 1.5 mm Screws, 60 mm length
128-1520-20	T8, for 2.0 / 2.4 mm screws, 60 mm length
128-2024-08	T8 for 2.0 / 2.4 mm screws, 100 mm length
128-2735-10	T10 for 2.7 / 3.5 mm screws, 100 mm length

**Screwdriver Handle**

Silicone, AO-Connection  
sterilizable up to 134°C / 273°F



Product Code	Description
247-0103-00	compact, compatible with 1.0/1.5/2.0/2.4
247-0102-00	standard, compatible with 2.7/3.5

**Torque Limiting Screwdriver Handle**

Torque 3 Nm  
Silicone, AO, sterilizable up to 134°C / 273°F



**247-0104-00**

# Osteosynthesis



## STANDARD PLATES

### 1.5mm DCP Plate

Cutttable

1mm thick, for 1.5 mm screws



Product Code	Holes	Length (mm)
130-1848-04	4	18.5
130-1848-05	5	22.5
130-1848-06	6	26.5
130-1848-07	7	30.5

Product Code	Holes	Length (mm)
130-1848-08	8	34.5
130-1848-09	9	38.5
130-1848-10	10	42.5
130-1848-20	20	82.5

### 2.0mm DCP Plate

1.5mm thick, 6.0mm wide



Product Code	Holes	Length (mm)
130-11-1014	4	27
130-11-1015	5	33
130-11-1016	6	39
130-11-1017	7	45

Product Code	Holes	Length (mm)
130-11-1018	8	51
130-11-1019	9	57
130-11-1020	10	63
130-11-1021	11	69
130-11-1022	12	75

### 2.4mm DCP Plate

2.0mm thick, 7.0mm wide



Product Code	Holes	Length (mm)
130-11-6004	4	32
130-11-6005	5	39
130-11-6006	6	46
130-11-6007	7	54
130-11-6008	8	61

Product Code	Holes	Length (mm)
130-11-6009	9	68
130-11-6010	10	75
130-11-6011	11	82
130-11-6012	12	89
130-11-6013	13	96
130-11-6014	14	103

### 2.7mm DCP Plate

2.5mm thick, 8.0mm wide



Product Code	Holes	Length (mm)
140-12-0004	4	37
140-12-0005	5	45
140-12-0006	6	53
140-12-0007	7	61
140-12-0008	8	70
140-12-0009	9	78

Product Code	Holes	Length (mm)
140-12-0010	10	86
140-12-0011	11	94
140-12-0012	12	102
140-12-0013	13	110
140-12-0014	14	118

## Plates (all)

## Bone Plate DCP 3.5

## 3.5mm DCP Plate narrow

4mm thick, 11mm wide, 5mm hole distance



Product Code	Holes	Length (mm)
140-20-0002	2	27
140-20-0004	4	51
140-20-0005	5	63
140-20-0006	6	75
140-20-0007	7	87
140-20-0008	8	99
140-20-0009	9	111
140-20-0010	10	123

Product Code	Holes	Length (mm)
140-20-0011	11	135
140-20-0012	12	147
140-20-0013	13	159
140-20-0014	14	171
140-20-0015	15	183
140-20-0016	16	195
140-20-0017	17	207
140-20-0018	18	219

## 3.5mm DCP Plate broad

5mm thick, 12.5mm wide, 5mm hole distance



Product Code	Holes	Length (mm)
140-24-0004	4	54
140-24-0005	5	66
140-24-0006	6	78
140-24-0007	7	90
140-24-0008	8	102
140-24-0009	9	114
140-24-0010	10	126
140-24-0011	11	138

Product Code	Holes	Length (mm)
140-24-0012	12	150
140-24-0013	13	162
140-24-0014	14	174
140-24-0015	15	186
140-24-0016	16	198
140-24-0017	17	210
140-24-0018	18	222
140-24-0019	19	234
140-24-0020	20	246



Online Shop

**veterinary**.shop

## Bone Plate DCP

### Bone Plate 4.5 mm DCP narrow



Product Code	Holes	Length (mm)
130-30-0004	4	71
130-30-0005	5	87
130-30-0006	6	103
130-30-0007	7	119
130-30-0008	8	135
130-30-0009	9	151
130-30-0010	10	167
130-30-0011	11	183
130-30-0012	12	199

Product Code	Holes	Length (mm)
130-30-0013	13	215
130-30-0014	14	231
130-30-0015	15	247
130-30-0016	16	263
130-30-0018	18	295
130-30-0020	20	327
130-30-0022	22	359
130-30-0024	24	391

### Bone Plate 4.5mm DCP broad



Product Code	Holes	Length (mm)
130-31-0005	5	87
130-31-0006	6	103
130-31-0007	7	119
130-31-0008	8	135
130-31-0009	9	151
130-31-0010	10	167
130-31-0011	11	183
130-31-0012	12	199

Product Code	Holes	Length (mm)
130-31-0013	13	215
130-31-0014	14	231
130-31-0015	15	247
130-31-0016	16	263
130-31-0018	18	295
130-31-0020	20	327
130-31-0022	22	359
130-31-0024	24	391

## Limited Contact DCP Plate

## Bone Plate Limited Contact

## 2.0mm Limited Contact DCP Plate



Product Code	Holes	Length (mm)
130-11-2004	4	23
130-11-2005	5	29
130-11-2006	6	35
130-11-2007	7	41

Product Code	Holes	Length (mm)
130-11-2008	8	47
130-11-2009	9	53
130-11-2010	10	59
130-11-2020	20	119

## 2.7 Limited Contact DCP Plate

Frontside



Backside (Limited Contact)



Product Code	Holes	Length (mm)
140-13-2004	4	36
140-13-2005	5	44
140-13-2006	6	52
140-13-2007	7	60
140-13-2008	8	68
140-13-2009	9	76

Product Code	Holes	Length (mm)
140-13-2010	10	84
140-13-2011	11	92
140-13-2012	12	100
140-13-2013	13	108
140-13-2014	14	116

## Bone Plate 3.5 mm Limited Contact DCP

Frontside



Backside (Limited Contact)



Product Code	Holes	Length (mm)
140-20-2004	4	51
140-20-2005	5	64
140-20-2006	6	77
140-20-2007	7	90
140-20-2008	8	103

Product Code	Holes	Length (mm)
140-20-2009	9	116
140-20-2010	10	129
140-20-2011	11	142
140-20-2012	12	155
140-20-2014	14	168

Acetabulum Plates



2,0mm, 6 Hole, 31mm

**130-11-0606**



2,7mm, 4 Hole, 39mm

**130-12-0604**



2,7mm, 5 Hole, 47mm

**130-12-0605**



2,7mm, 6 Hole, 53mm

**130-12-0606**

Reconstruction Plates 3.5mm

Straight



Product Code	Holes	Length (mm)
140-50-0004	4	46
140-50-0005	5	58
140-50-0006	6	70
140-50-0007	7	82
140-50-0008	8	94
140-50-0009	9	106
140-50-0010	10	118

Product Code	Holes	Length (mm)
140-50-0011	11	130
140-50-0012	12	142
140-50-0014	14	166
140-50-0016	16	190
140-50-0018	18	214
140-50-0020	20	238
140-50-0022	22	262

Reconstruction Plates 3.5mm

Curved



Product Code	Holes	Length (mm)
130-50-0106	6	48
130-50-0108	8	64
130-50-0110	10	80

Product Code	Holes	Length (mm)
130-50-0112	12	96
130-50-0114	14	112
130-50-0116	16	128

2.0mm Adaption Plate

20 holes, 1.2 mm thickness, cuttable



**130-11-1420**

T-Plate, standard

L-Plate, standard

2.0mm T-Bone Plate

2x2 holes, 1.0mm thick, 5.0mm wide, 6mm hole distance

130-11-0302



1.5mm T-Plate (cuttable)

Product Code	Holes	Length (mm)
130-1863-09	3x9	50
130-1864-09	4x9	50



2.0mm T-Plate (cuttable)

Product Code	Holes	Length (mm)
130-11-0339	3x9	50
130-11-0349	4x9	50



2.0mm T-Plate

Product Code	Holes	Length (mm)
140-0620-24	2x4	32
140-0620-25	2x5	38
140-0620-26	2x6	44



Product Code	Holes	Length (mm)
140-0620-27	2x7	50
140-0620-28	2x8	56

2.0 mm L-Plate

Product Code	Description
130-11-0402	left
130-11-0502	right



2.7 mm L-Plate

Product Code	Description
130-12-0103	left
130-12-0203	right



Phillips T-Plates



Product Code	Holes	Dimensions
131-20-0304	2/4	2.0/2.7 mm, 36 mm
131-20-0305	2/5	2.0/2.7 mm, 44 mm
131-20-0306	2/6	2.0/2.7 mm, 52 mm

3.5 mm T - Bone Plate



Product Code	Holes	Dimensions
131-35-0505	2/5	3.5/65 mm
131-35-0506	2/6	3.5/75 mm

3.5 mm T - Bone Plate with curved head



Product Code	Holes	Dimensions
131-35-0404	3/4	3.5/60 mm
131-35-0406	3/6	3.5/80 mm
131-35-0508	3/8	3.5/105 mm

Arthrodesis Plates

Product Code Description

140-05-1168 9 holes oval, 1.5/2.0/54 mm



140-05-1169 9 holes oval, 2.0/2.0/58 mm



140-05-1170 9 holes round, 2.0/2.7/76 mm



140-05-1171 9 holes oval, 2.0/2.7/76 mm



140-05-1172 9 holes round, 2.7/3.5/120 mm



140-05-1173 9 holes oval, 2.7/3.5/120 mm



140-05-1174 9 holes round, 2.7/3.5/104 mm



140-05-1175 9 holes oval, 2.7/3.5/104 mm



140-06-1176 11 holes oval, 3.5/3.5/152 mm




140-05-1177 10 holes round, 3.5/3.5/140 mm



140-06-1178 10 holes oval, 3.5/3.5/140 mm



# Osteosynthesis

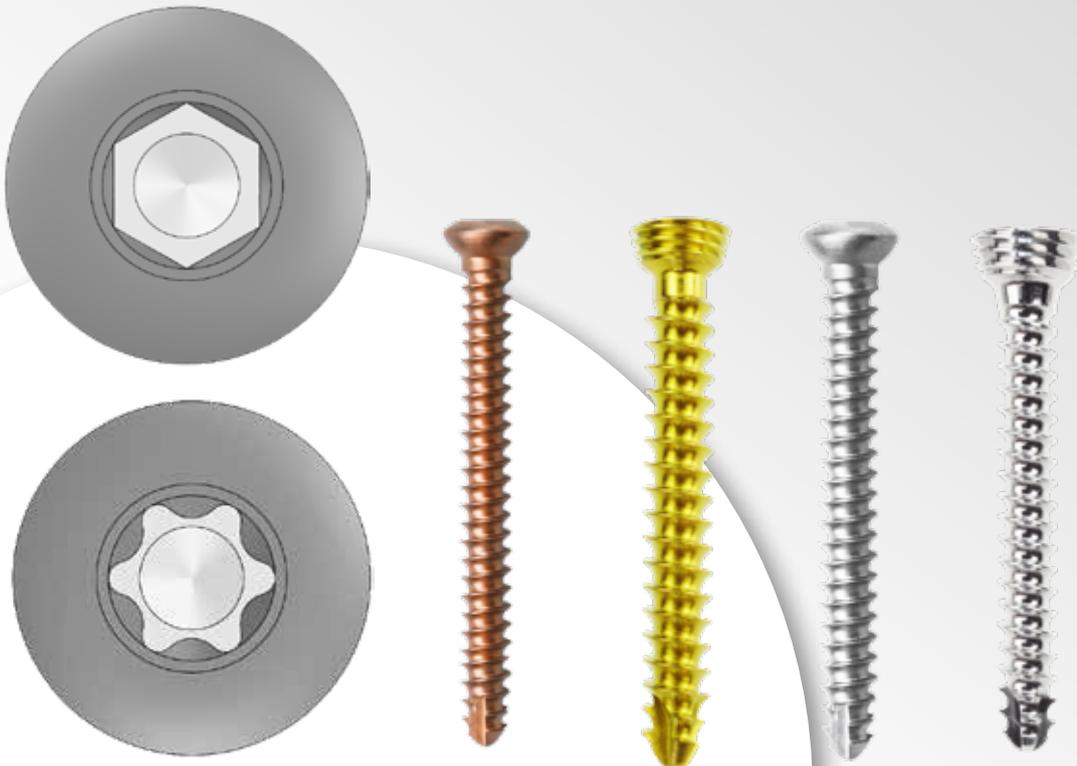

## SCREWS

## Cortical Screws (All)

**1.5 mm Cortical Screw** Hexagonal or LeiStar head, self-holding, self-tapping with three flute cutting edge



Length (mm)	Stainless		Titanium	
	Hex Head	LeiStar	Hex Head	LeiStar
5				245-515-05
6	245-115-06		245-215-06	245-515-06
7	245-115-07		245-215-07	245-515-07
8	245-115-08		245-215-08	245-515-08
9	245-115-09		245-215-09	245-515-09
10	245-115-10		245-215-10	245-515-10
11	245-115-11		245-215-11	
12	245-115-12		245-215-12	245-515-12
14	245-115-14		245-215-14	245-515-14
16	245-115-16		245-215-16	245-515-16
18	245-115-18		245-215-18	245-515-18
20	245-115-20		245-215-20	245-515-20

**2.0mm Cortical Screw** Hexagonal or LeiStar head, self-holding, self-tapping with three flute cutting edge



Length (mm)	Stainless		Titanium	
	Hex Head	LeiStar	Hex Head	LeiStar
5				245-520-05
6	245-120-06	245-620-06	245-220-06	245-520-06
7				245-520-07
8	245-120-08	245-620-08	245-220-08	245-520-08
9				245-520-09
10	245-120-10	245-620-10	245-220-10	245-520-10
12	245-120-12	245-620-12	245-220-12	245-520-12
14	245-120-14	245-620-14	245-220-14	245-520-14
16	245-120-16	245-620-16	245-220-16	245-520-16
18	245-120-18	245-620-18	245-220-18	245-520-18
20	245-120-20	245-620-20	245-220-20	245-520-20
22	245-120-22	245-620-22	245-220-22	245-520-22
24	245-120-24	245-620-24	245-220-24	245-520-24
26	245-120-26	245-620-26	245-220-26	245-520-26
28	245-120-28	245-620-28	245-220-28	245-520-28
30	245-120-30	245-620-30	245-220-30	245-520-30
32	245-120-32	245-620-32		
34	245-120-34	245-620-34		
36	245-120-36	245-620-36		
38	245-120-38	245-620-38		
40	245-120-40	245-620-40		
42	245-120-42			
44	245-120-44			

## 2.4 mm Cortical Screw Hexagonal or LeiStar head, self-holding, self-tapping with three flute cutting edge



Length (mm)	Stainless		Titanium	
	Hex Head	LeiStar	Hex Head	LeiStar
6	245-124-06	245-624-06	245-224-06	245-524-06
8	245-124-08	245-624-08	245-224-08	245-524-08
10	245-124-10	245-624-10	245-224-10	245-524-10
12	245-124-12	245-624-12	245-224-12	245-524-12
14	245-124-14	245-624-14	245-224-14	245-524-14
16	245-124-16	245-624-16	245-224-16	245-524-16
18	245-124-18	245-624-18	245-224-18	245-524-18
20	245-124-20	245-624-20	245-224-20	245-524-20
22	245-124-22	245-624-22	245-224-22	245-524-22
24	245-124-24	245-624-24	245-224-24	245-524-24
26	245-124-26	245-624-26	245-224-26	245-524-26
28	245-124-28	245-624-28	245-224-28	245-524-28
30	245-124-30	245-624-30	245-224-30	245-524-30
32	245-124-32	245-624-32	245-224-32	245-524-32
34	245-124-34	245-624-34	245-224-34	245-524-34
36	245-124-36	245-624-36	245-224-36	245-524-36
38	245-124-38	245-624-38	245-224-38	245-524-38
40	245-124-40	245-624-40	245-224-40	245-524-40

## 2.7 mm Cortical Screw Hexagonal or LeiStar head, self-holding, self-tapping with three flute cutting edge



Length (mm)	Stainless		Titanium	
	Hex Head	LeiStar	Hex Head	LeiStar
6	245-127-06		245-227-06	245-527-06
8	245-127-08		245-227-08	245-527-08
10	245-127-10	245-627-10	245-227-10	245-527-10
12	245-127-12	245-627-12	245-227-12	245-527-12
14	245-127-14	245-627-14	245-227-14	245-527-14
16	245-127-16	245-627-16	245-227-16	245-527-16
18	245-127-18	245-627-18	245-227-18	245-527-18
20	245-127-20	245-627-20	245-227-20	245-527-20
22	245-127-22	245-627-22	245-227-22	245-527-22
24	245-127-24	245-627-24	245-227-24	245-527-24
26	245-127-26	245-627-26	245-227-26	245-527-26
28	245-127-28	245-627-28	245-227-28	245-527-28
30	245-127-30	245-627-30	245-227-30	245-527-30
32	245-127-32	245-627-32	245-227-32	245-527-32
34	245-127-34	245-627-34	245-227-34	245-527-34
36	245-127-36	245-627-36	245-227-36	245-527-36
38	245-127-38	245-627-38	245-227-38	245-527-38
40	245-127-40	245-627-40	245-227-40	245-527-40
42	245-127-42			
45				245-527-45
50				245-527-50



## Washers

### 3.5 Cortical Screw (Non-Locking) Stainless Steel

Hexagonal or LeiStar head,  
self-holding (T10 Shaft from Rita Leibinger needed)  
self-tapping with three flute cutting edge



Length (mm)	Stainless		Titanium	
	Hex Head	LeiStar	Hex Head	LeiStar
8	245-135-08	245-635-08	245-235-08	245-535-08
10	245-135-10	245-635-10	245-235-10	245-535-10
12	245-135-12	245-635-12	245-235-12	245-535-12
14	245-135-14	245-635-14	245-235-14	245-535-14
16	245-135-16	245-635-16	245-235-16	245-535-16
18	245-135-18	245-635-18	245-235-18	245-535-18
20	245-135-20	245-635-20	245-235-20	245-535-20
22	245-135-22	245-635-22	245-235-22	245-535-22
24	245-135-24	245-635-24	245-235-24	245-535-24
26	245-135-26	245-635-26	245-235-26	245-535-26
28	245-135-28	245-635-28	245-235-28	245-535-28
30	245-135-30	245-635-30	245-235-30	245-535-30
32	245-135-32	245-635-32	245-235-32	245-535-32
34	245-135-34	245-635-34	245-235-34	245-535-34
36	245-135-36	245-635-36	245-235-36	245-535-36
38	245-135-38	245-635-38	245-235-38	245-535-38
40	245-135-40	245-635-40	245-235-40	245-535-40
42	245-135-42			
44	245-135-44			
45	245-135-45	245-635-45	245-235-45	245-535-45
50	245-135-50	245-635-50	245-235-50	245-535-50
55	245-135-55	245-635-55	245-235-55	245-535-55
60	245-135-60	245-635-60	245-235-60	245-535-60
65	245-135-65			

### Washers

Stainless Steel

Product Code	Description
130-5215-10	Washer 1.5
130-6252-12	Washer 2.0
130-7324-14	Washer 2.4
130-8327-16	Washer 2.7
130-9435-16	Washer 3.5



### 4.0 mm Cancellous Screws

Hexagonal head,  
 self-holding, self-tapping with three flute cutting edge



Length (mm)	Fully Threaded	Partially Threaded
10	245-440-10	245-140-10
12	245-440-12	245-140-12
14	245-440-14	245-140-14
16	245-440-16	245-140-16
18	245-440-18	245-140-18
20	245-440-20	245-140-20
22	245-440-22	245-140-22
24	245-440-24	245-140-24
26	245-440-26	245-140-26
28	245-440-28	245-140-28
30	245-440-30	245-140-30
32	245-440-32	245-140-32
34	245-440-34	245-140-34
35	245-440-35	245-140-35
36	245-440-36	245-140-36
38	245-440-38	245-140-38
40	245-440-40	245-140-40
42	245-440-42	245-140-42
44	245-440-44	245-140-44
45		245-140-45
46	245-440-46	245-140-46
48	245-440-48	245-140-48
50	245-440-50	245-140-50
52	245-440-52	245-140-52
54	245-440-54	245-140-54
55	245-440-55	245-140-55
56	245-440-56	245-140-56
58	245-440-58	245-140-58
60	245-440-60	245-140-60
62	245-440-62	245-140-62
63	245-440-64	245-140-64
66	245-440-66	245-140-66
68	245-440-68	245-140-68
70	245-440-70	245-140-70

### 4.5 mm Cortical Screw

Hexagonal head,  
 self-holding, self-tapping with three flute cutting edge



Length (mm)	Stainless Steel
14	245-145-14
16	245-145-16
18	245-145-18
20	245-145-20
22	245-145-22
24	245-145-24
26	245-145-26
28	245-145-28
30	245-145-30
32	245-145-32
34	245-145-34
36	245-145-36
38	245-145-38
40	245-145-40
42	245-145-42
44	245-145-44
46	245-145-46
48	245-145-48
50	245-145-50
52	245-145-52
54	245-145-54
56	245-145-56
58	245-145-58
60	245-145-60
62	245-145-62
64	245-145-64
66	245-145-66
68	245-145-68
70	245-145-70



## Locking Screws (All)

### Locking Screws Titanium

For **LeiLOX Osteosynthesis Locking Systems and C-LOX (2.7mm)**

LeiStar

self-holding (Shafts from Rita Leibinger recommended)

self-tapping with three flute cutting edge



**STAR** Screw-Head



**LeiLOX Osteosynthesis Systems**

**C-LOX**

Length (mm)	LeiLOX Osteosynthesis Systems				C-LOX
	Nano		Micro		
	1.0 mm	1.3 mm	1.5 mm	2.0 mm	2.7 mm
	Product Code	Product Code	Product Code	Product Code	Product Code
4	245-410-04	245-413-04			
5	245-410-05	245-413-05	245-415-05	245-420-05	
6	245-410-06	245-413-06	245-415-06	245-420-06	
7	245-410-07	245-413-07	245-415-07	245-420-07	
8	245-410-08	245-413-08	245-415-08	245-420-08	245-427-08
9	245-410-09	245-413-09	245-415-09	245-420-09	
10	245-410-10	245-413-10	245-415-10	245-420-10	245-427-10
11	245-410-11	245-413-11	245-415-11	245-420-11	
12	245-410-12	245-413-12	245-415-12	245-420-12	245-427-12
14	245-410-14	245-413-14	245-415-14	245-420-14	245-427-14
16	245-410-16	245-413-16	245-415-16	245-420-16	245-427-16
18		245-413-18	245-415-18	245-420-18	245-427-18
20		245-413-20	245-415-20	245-420-20	245-427-20
22			245-415-22	245-420-22	
24			245-415-24	245-420-24	
26			245-415-26	245-420-26	
28				245-420-28	
30				245-420-30	

### 2.0 / 2.4 LeiLOX Locking Screw Titanium

For LeiLOX Locking **TPLO, CBLO, CCWO Systems**  
 LeiStar T8  
 self-holding (Shafts from Rita Leibinger recommended)  
 self-tapping with three flute cutting edge



	2.0 mm	2.4 mm
Length (mm)	Product Code	Product Code
06	242-220-06	242-224-06
08	242-220-08	242-224-08
10	242-220-10	242-224-10
12	242-220-12	242-224-12
14	242-220-14	242-224-14
16	242-220-16	242-224-16
18	242-220-18	242-224-18
20	242-220-20	242-224-20
22	242-220-22	242-224-22
24	242-220-24	242-224-24
26	242-220-26	242-224-26
28	242-220-28	242-224-28
30	242-220-30	242-224-30
32		242-224-32
34		242-224-34
36		242-224-36
38		242-224-38
40		242-224-40

### 2.7 / 3.5 LeiLOX Locking Screw Titanium

For LeiLOX Locking **TPLO, CBLO, CCWO Systems**  
 LeiStar T10  
 self-holding (Shafts from Rita Leibinger recommended)  
 self-tapping with three flute cutting edge



	2.7 mm	3.5 mm
Length (mm)	Product Code	Product Code
10	242-227-10	242-235-10
12	242-227-12	242-235-12
14	242-227-14	242-235-14
16	242-227-16	242-235-16
18	242-227-18	242-235-18
20	242-227-20	242-235-20
22	242-227-22	242-235-22
24	242-227-24	242-235-24
26	242-227-26	242-235-26
28	242-227-28	242-235-28
30	242-227-30	242-235-30
32	242-227-32	242-235-32
34	242-227-34	242-235-34
36	242-227-36	242-235-36
38	242-227-38	242-235-38
40	242-227-40	242-235-40
42	242-227-42	242-235-42
44	242-227-44	242-235-44
46	242-227-46	242-235-46
48	242-227-48	242-235-48
50	242-227-50	242-235-50
52		242-235-52
54		242-235-54
56		242-235-56
58		242-235-58
60		242-235-60



## LeiLOX Locking Screws Stainless Steel

### LeiLOX Locking Screws Stainless Steel

For LeiLOX Osteosynthesis Locking Systems and TPLO

LeiStar , T8 (2.0/2.4) & T10 (2.7/3.5)

self-holding (Shafts from Rita Leibinger recommended)

self-tapping with three flute cutting edge



Length (mm)	2.0 mm	2.4 mm	2.7 mm	3.5 mm
	Product Code	Product Code	Product Code	Product Code
6	242-120-06	242-124-06		
8	242-120-08	242-124-08		
10	242-120-10	242-124-10	242-127-10	242-135-10
12	242-120-12	242-124-12	242-127-12	242-135-12
14	242-120-14	242-124-14	242-127-14	242-135-14
16	242-120-16	242-124-16	242-127-16	242-135-16
18	242-120-18	242-124-18	242-127-18	242-135-18
20	242-120-20	242-124-20	242-127-20	242-135-20
22	242-120-22	242-124-22	242-127-22	242-135-22
24	242-120-24	242-124-24	242-127-24	242-135-24
26	242-120-26	242-124-26	242-127-26	242-135-26
28	242-120-28	242-124-28	242-127-28	242-135-28
30	242-120-30	242-124-30	242-127-30	242-135-30
32		242-124-32	242-127-32	242-135-32
34		242-124-34	242-127-34	242-135-34
36		242-124-36	242-127-36	242-135-36
38		242-124-38	242-127-38	242-135-38
40		242-124-40	242-127-40	242-135-40
42			242-127-42	242-135-42
44			242-127-44	242-135-44
46			242-127-46	242-135-46
48			242-127-48	242-135-48
50			242-127-50	242-135-50
52				242-135-52
54				242-135-54
56				242-135-56
58				242-135-58
60				242-135-60
62				242-135-62
64				242-135-64
66				242-135-66
68				242-135-68
70				242-135-70

# Osteosynthesis

K-Wires

Osteosynthesis  
General



## K-WIRES

**R** RITA  
LEIBINGER  
MEDICAL

## K-Wire Set

### K-Wire Set

111-0015-10



The K-Wires contained in the set are single trocars with round ends.

The set contains:

Product Code	Description	Qty
150-0865-00	Tray with Lid for K-Wires	1
143-1000-04	Cerclage Wire, 0,4 mm, 10m roll	1
143-1000-06	Cerclage Wire, 0,6 mm, 10m roll	1
143-1000-08	Cerclage Wire, 0,8 mm, 10m roll	1
143-1000-10	Cerclage Wire, 1,0 mm, 10m roll	1
144-1010-10	1.0mm x 100mm (CCC) K-Wire	6
144-1010-15	1.0mm x 150mm (CCC) K-Wire	6
144-1010-20	1.0mm x 200mm (CCC) K-Wire	6
144-1015-10	1.5mm x 100mm (CCC) K-Wire	6
144-1015-15	1.5mm x 150mm (CCC) K-Wire	6
144-1015-20	1.5mm x 200mm (CCC) K-Wire	6
144-1020-10	2.0mm x 100mm (CCC) K-Wire	6
144-1020-15	2.0mm x 150mm (CCC) K-Wire	6
144-1020-20	2.0mm x 200mm (CCC) K-Wire	6
144-1025-10	2.5mm x 100mm (CCC) K-Wire	6
144-1025-15	2.5mm x 150mm (CCC) K-Wire	6
144-1025-20	2.5mm x 200mm (CCC) K-Wire	6




### Sterilization Container

See Sterilization Containers for Implants and Instruments Trays on **Page 204**.

**K-Wire Instrument Set**

111-0015-20

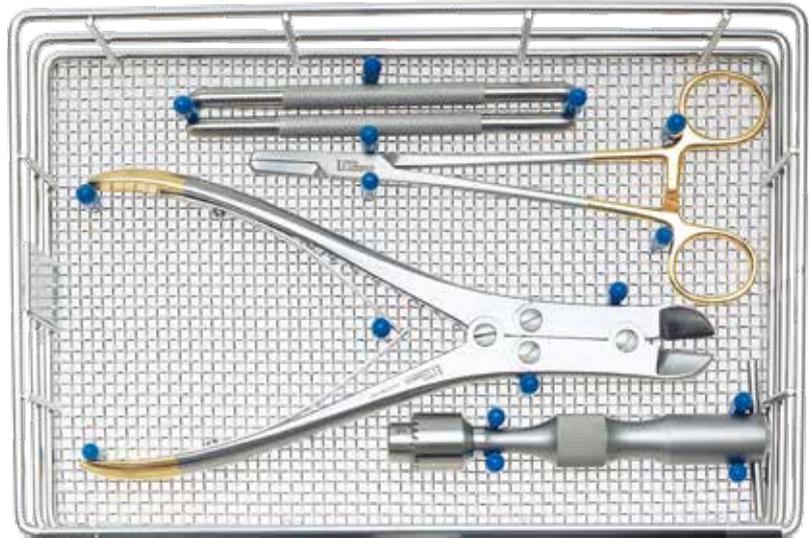

The set contains:

Product Code	Description
150-0866-00	Instrument Tray for K-Wire Set
23-3513-00	Hand Chuck and key, max. Ø 4 mm
23-1363-14	K- Wire Bender, 1.0/2.0 mm 14 cm
23-1364-14	K-Wire Bender, 1.5/2.5mm, 14 cm
23-5795-22T	Wirecutter TC, 22 cm, for wires up to 2,6 mm
23-5535-18T	Wire Twister Berry, 18,5cm ,7 1/4", straight



[www.LEIBINGER-MEDICAL.com](http://www.LEIBINGER-MEDICAL.com)

**Orthopedic Cerclage**

Wires 10 meter roll



**INFO:** More sizes available upon request

Ø (mm)	Product Code
0.2	143-1000-02
0.3	143-1000-03
0.4	143-1000-04
0.5	143-1000-05
0.6	143-1000-06
0.7	143-1000-07

Ø (mm)	Product Code
0.8	143-1000-08
0.9	143-1000-09
1.0	143-1000-10
1.2	143-1000-12
1.5	143-1000-15

## K-Wires

### Single Trocar

Rounded end

Sold in packs of 10 for sizes up to 3.0 and in packs of 5 from size 3.5 upwards

**INFO:** More sizes available upon request

	Size (mm)		Product Code
	Ø	L	
K-Wire	0.8	100	144-1008-10
		150	144-1008-15
		300	144-1008-20
	1.0	100	144-1010-10
		150	144-1010-15
		300	144-1010-30
	1.2	100	144-1012-10
		150	144-1012-15
		200	144-1012-20
	1.4	100	144-1014-10
		150	144-1014-15
		200	144-1014-20
1.5	100	144-1015-10	
	150	144-1015-15	
	200	144-1015-20	
	250	144-1015-25	
	300	144-1015-30	
1.6	100	144-1016-10	
	150	144-1016-15	
	200	144-1016-20	
	250	144-1016-25	
	300	144-1016-30	

	Size (mm)		Product Code
	Ø	L	
K-Wire	1.8	100	144-1018-10
		150	144-1018-15
		200	144-1018-20
		250	144-1018-25
		300	144-1018-30
	2.0	100	144-1020-10
Steinmann Pin	2.0	150	144-1020-15
		200	144-1020-20
		250	144-1020-25
	2.5	300	144-1020-30
		100	144-1025-10
		150	144-1025-15
3.0	200	144-1025-20	
	250	144-1025-25	
	300	144-1025-30	
	100	144-1030-10	
	150	144-1030-15	
200	144-1030-20		
250	144-1030-25		
300	144-1030-30		

	Size (mm)		Product Code
	Ø	L	
Steinmann Pin	3.5	100	144-1035-10
		150	144-1035-15
		200	144-1035-20
		250	144-1035-25
		300	144-1035-30
	4.0	100	144-1040-10
		150	144-1040-15
		200	144-1040-20
		250	144-1040-25
		300	144-1040-30
	4.5	150	144-1045-15
		200	144-1045-20
		250	144-1045-25
		300	144-1045-30
		5.0	150
200	144-1050-20		
250	144-1050-25		
300	144-1050-30		
6.0	150		144-1060-15
	200	144-1060-20	
	250	144-1060-25	
	300	144-1060-30	

### Single Trocar, threaded (negative)

Rounded end, with 15 mm negative threaded tip

Sold in packs of 10 for sizes up to 3.0 and in packs of 5 from size 3.5 upwards

**INFO:** More sizes available upon request

	Size (mm)		Product Code
	Ø	L	
K-Wire	1.0	100	144-1510-10
		150	144-1510-15
		200	144-1510-20
		250	144-1510-25
		300	144-1510-30
	1.2	100	144-1512-10
		150	144-1512-15
		200	144-1512-20
		250	144-1512-25
		300	144-1512-30

	Size (mm)		Product Code
	Ø	L	
K-Wire	1.4	100	144-1514-10
		150	144-1514-15
		200	144-1514-20
		250	144-1514-25
		300	144-1514-30
	1.5	100	144-1515-10
		150	144-1515-15
		200	144-1515-20
		250	144-1515-25
		300	144-1515-30

	Size (mm)		Product Code
	Ø	L	
K-Wire	1.6	100	144-1516-10
		150	144-1516-15
		200	144-1516-20
		250	144-1516-25
		300	144-1516-30
	1.8	100	144-1518-10
		150	144-1518-15
		200	144-1518-20
		250	144-1518-25
		300	144-1518-30
	2.0	100	144-1520-10
		150	144-1520-15
		200	144-1520-20
		250	144-1520-25
		300	144-1520-30

**Single Trocar, threaded (negative)**

Rounded end, with 15 mm negative threaded tip

Sold in packs of 10 for sizes up to 3.0 and in packs of 5 from size 3.5 upwards



	Size (mm)		Product Code
	Ø	L	
Steinmann Pin	2.5	100	144-1525-10
		150	144-1525-15
		200	144-1525-20
		250	144-1525-25
		300	144-1525-30
	3.0	100	144-1530-10
		150	144-1530-15
		200	144-1530-20
		250	144-1530-25
		300	144-1530-30

	Size (mm)		Product Code
	Ø	L	
Steinmann Pin	3.5	150	144-1535-15
		200	144-1535-20
		250	144-1535-25
		300	144-1535-30
		4.0	150
	200		144-1540-20
	250		144-1540-25
	300		144-1540-30

INFO: More sizes available upon request

	Size (mm)		Product Code
	Ø	L	
Steinmann Pin	4.5	150	144-1516-15
		200	144-1516-20
		250	144-1516-25
		300	144-1516-30
	5.0	150	144-1518-15
		200	144-1518-20
		250	144-1518-25
		300	144-1518-30
	6.0	150	144-1520-15
		200	144-1520-20
		250	144-1520-25
		300	144-1520-30

**Double Trocar**

Sold in packs of 10 for sizes up to 3.0 and in packs of 5 from size 3.5 upwards



	Size (mm)		Product Code
	Ø	L	
K-Wire	0.8	100	144-2008-10
		150	144-2008-15
		300	144-2008-20
	1.0	100	144-2010-10
		150	144-2010-15
		200	144-2010-20
		250	144-2010-25
		300	144-2010-30
	1.2	100	144-2012-10
		150	144-2012-15
		200	144-2012-20
		250	144-2012-25
		300	144-2012-30
	1.4	100	144-2014-10
		150	144-2014-15
		200	144-2014-20
		250	144-2014-25
		300	144-2014-30
	1.5	100	144-2015-10
		150	144-2015-15
200		144-2015-20	
250		144-2015-25	
300		144-2015-30	

	Size (mm)		Product Code
	Ø	L	
K-Wire	1.6	100	144-2016-10
		150	144-2016-15
		200	144-2016-20
		250	144-2016-25
		300	144-2016-30
	1.8	100	144-2018-10
		150	144-2018-15
		200	144-2018-20
		250	144-2018-25
		300	144-2018-30
	2.0	100	144-2020-10
		150	144-2020-15
		200	144-2020-20
		250	144-2020-25
		300	144-2020-30

	Size (mm)		Product Code
	Ø	L	
Steinmann Pin	2.5	100	144-2025-10
		150	144-2025-15
		200	144-2025-20
		250	144-2025-25
		300	144-2025-30
	3.0	100	144-2030-10
		150	144-2030-15
		200	144-2030-20
		250	144-2030-25
		300	144-2030-30

	Size (mm)		Product Code
	Ø	L	
Steinmann Pin	3.5	150	144-2035-15
		200	144-2035-20
		250	144-2035-25
		300	144-2035-30
		4.0	150
	200		144-2040-20
	250		144-2040-25
	300		144-2040-30
	4.5		150
		200	144-2045-20
		250	144-2045-25
		300	144-2045-30
		5.0	150
	200		144-2050-20
	250		144-2050-25
	300		144-2050-30
	6.0		150
		200	144-2060-20
		250	144-2060-25
		300	144-2060-30

INFO: More sizes available upon request

# LeiMESH

## Cuttable Mesh Plate System


### Three-Dimensional Adaptability

The Titanium LeiMESH features a unique geometric pattern design. This creates a flexible structure that can be easily bent and shaped, which is essential for creating a custom fit during surgery. It becomes more rigid when formed into a three dimensional configuration, providing stable support.




### Titanium for Best Biocompatibility

Made of medical grade Titanium, LeiMESH is highly biocompatible, strong yet lightweight, corrosion-resistant, and promotes bone integration. Its flexibility makes it suitable for custom shaping and its non-magnetic properties makes it safe for MRI scans.

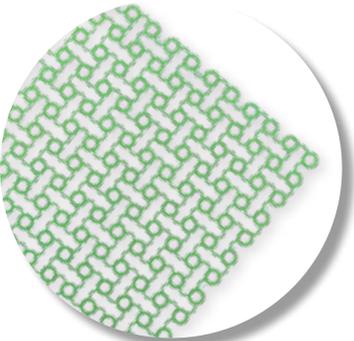

### Perfect Balance of Strength and Flexibility

The thickness of LeiMESH provides sufficient structural support while allowing flexibility to customize the mesh to fit complex contours.

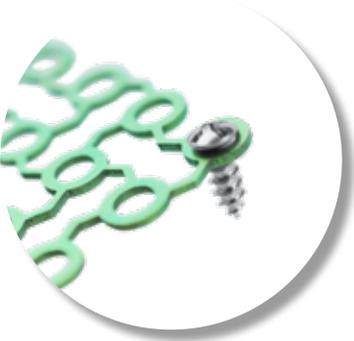

### Various Applications

LeiMESH is highly versatile and can be used in various medical applications such as cranial fracture repair, bone fracture management, bone cement augmentation, and maxillofacial reconstruction surgeries.



### Low Profile Cross Drive Titanium Screws

Made of Titanium to ensure seamless biocompatibility, LeiMESH Screws feature a low-profile head for minimal tissue irritation. Compatible with the LeiMESH Screwdriver, the LeiMESH Cross Drive screws provide a secure fixation, fitting perfectly into the screw holes of the Titanium Mesh to meet diverse anatomical and surgical requirements. Additionally, they offer a self-holding capability similar to LeiStar screws.



# LeiMESH



## DYNAMIC MESH SYSTEM

**R** RITA  
LEIBINGER  
MEDICAL

## LeiMESH 3D Dynamic Mesh Set

### LeiMESH 3D Dynamic Mesh Set


Contains:

- 1 LeiMESH 3D Dynamic Titanium Mesh
- 5 of each LeiMESH Titanium Screws  
(Ø 1.6 mm, Lengths: 4 - 8 mm // 25 total)
- 1 LeiMESH Screwdriver Handle
- 1 LeiMESH Screwdriver Shaft
- 1 of each Micro Twist Bone Drill  
(Ø 1.0 mm, Drill Lengths: 3 mm, 5 mm, 8 mm)
- Universal Wire Scissors
- 1 Tray for LeiMESH Set with Lid

**141-9090-00**

Tray without contents

**141-9090-10**

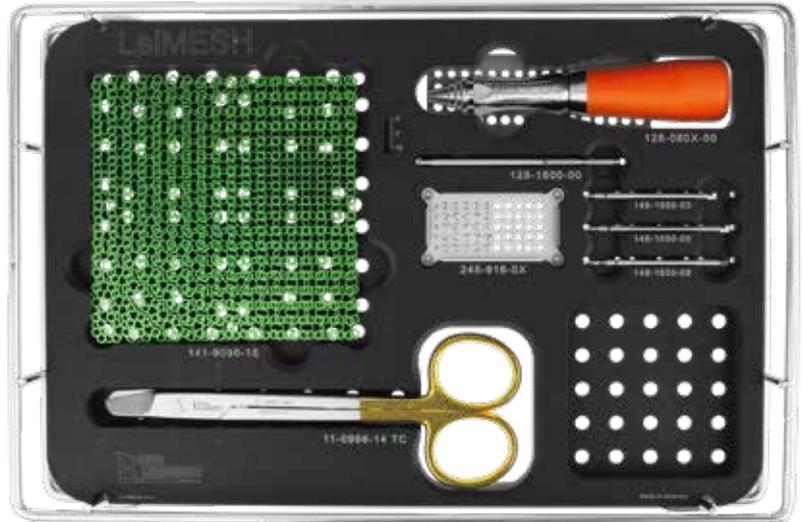

### Bending Pliers with Tray



Contains:

- 1 LeiMESH Bending Pliers
- 1 Tray (without lid)

**141-9091-00**

Tray without lid and contents

**141-9091-10**

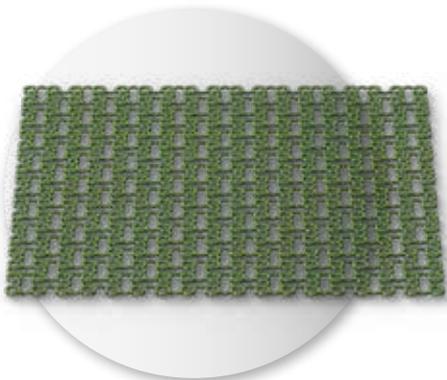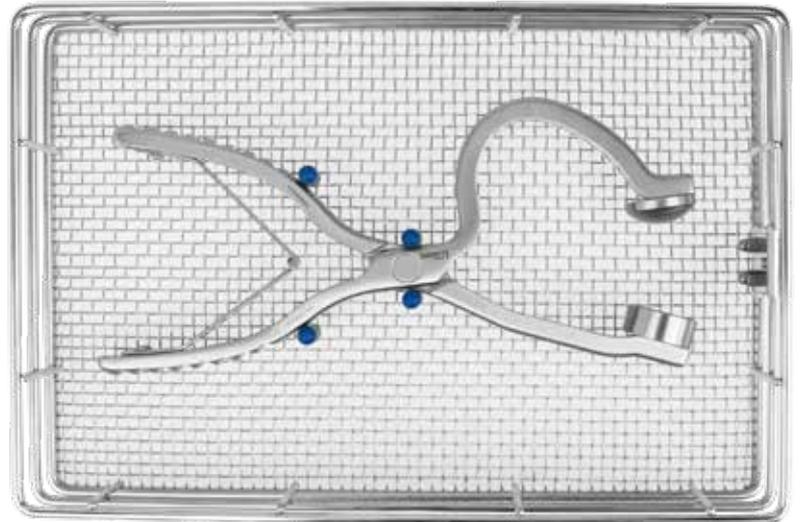

**NEW**

### LeiMESH Cuttable Titanium Mesh System

Composed of high-quality titanium, LeiMESH offers surgeons the flexibility to shape implants during surgery.

LeiMESH Implants provide a unique solution for treating cranial or maxillofacial fractures after trauma, reconstruction after tumors, as well as mandibular cases.

LeiMESH Implants are ideal for osteosynthesis in non-load-bearing bones.

LeiMESH Implants are used to augment bone cement in joint replacement procedures.

LeiMESH Implants offer the dual benefits of exceptional biocompatibility and superior corrosion resistance.

LeiMESH Implants are suitable for permanent implantation in animals due to their long-term stability.


LeiMESH Cuttable Mesh Titanium

LeiMESH System Instruments

**3D Dynamic Cuttable Mesh Titanium**

0.6 mm thick, 90 mm x 90 mm

**141-9090-15**

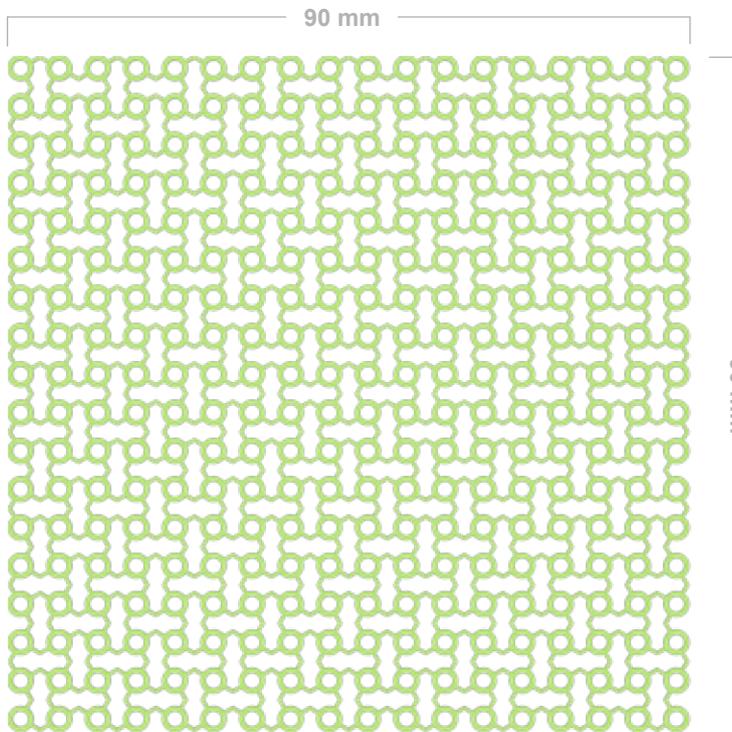

**LeiMESH Screw Titanium**

Ø 1.6 mm, low profile, Cross Drive



Product Code	Length (mm)
245-916-04	4
245-916-05	5
245-916-06	6
245-916-07	7
245-916-08	8

**LeiMESH Screwdriver Handle**

with dental connector/coupler

**128-0803-00**



**LeiMESH Micro Twist Bone Drill**

Ø 1.0 mm, with dental connector/coupler



Product Code	Drill Length
148-1050-03	3 mm
148-1050-05	5 mm
148-1050-08	8 mm

**Universal Wire Scissors**

Stainless Steel

**11-0966-14TC**



**LeiMESH Screwdriver Shaft**

Cross Drive, with dental connector/coupler

**128-1600-00**




**LeiMESH Bending Pliers**

Stainless Steel

**128-0122-25**



# LeiCOM Cannulated Compression Bone Screws

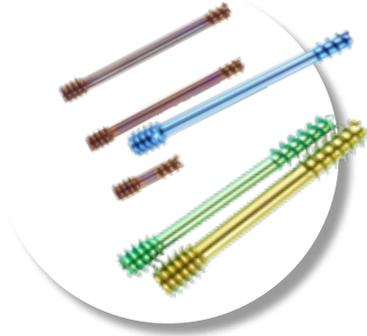

## Titanium Compression Bone Screw Systems for small animals

The LeiCOM Cannulated Compression Bone Screws create compression through different thread pitches at the head of the screw and at the distal thread of the screw. Available in Micro, Mini, Medium and Maxi sizes, our compression screws offer a solution for every need - from small to large breeds.



## Titanium: Best Biocompatibility

Unique Titanium Alloy makes our compression screws very durable but lightweight. Titanium is also highly biocompatible and has low temperature sensitiveness.



## Improved Accuracy and Optimized Positioning

All screws are cannulated to allow placement over a guidewire ensuring better accuracy before drilling or screw insertion. Using cannulated screws adopts the principles of interfragmentary screw fixation and aims to optimize screw position.



## Various Applications

The LeiCOM Cannulated Compression Bone Screws can be used for corrective osteotomies, fracture fixations, distal femur, humeral condyle, degenerative changes in small bone, and non-unions.

## LeiStar Compression Screws

All of our cannulated compression screws have LeiStar screwheads, which allows for better tightening torque compared to other screwheads. The screwdriver shaft is self-holding and keeps the screws firmly on the driver.



# LeiCOM



Special Thanks to  
Dr. Yves Samoy

## COMPRESSION SCREWS

**R** RITA  
LEIBINGER  
MEDICAL

# LEICOM CANNULATED COMPRESSION SCREWS

## Surgical Protocol

### Application

The RITA LEIBINGER LeiCOM Cannulated Compression Screws have the versatility to be utilized either as standalone implants or with K-Wires.

### Indications

Fractures, corrective osteotomy, pseudoarthrosis, degenerative bone changes, fractures of the humeral condyle, fractures of the distal femur.

### Surgical Technique



**1**  
Temporary fixation using a K-Wire (guide wire).



**2**  
The RITA LEIBINGER LeiCOM Compression Screws are self-tapping. However, in case of thick cortical bone, we recommend drilling to the core diameter to make it easier to insert the compression screw. Drill over the K-Wire with the cannulated twist drill.




**3**  
To ensure optimal insertion of the screw/thread head, use of the cannulated screw head countersink is recommended.



**4**  
The screw length is determined using the screw depth gauge over the K-wire into the bone.

**IMPORTANT:** To prevent the counter cortex from breaking through, the next smaller screw length is recommended.

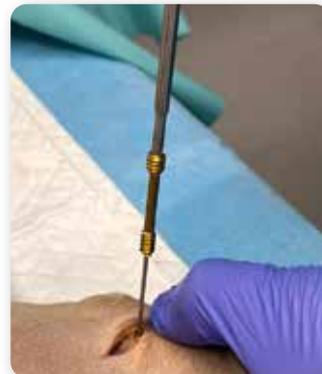

**5**  
The compression screw is placed over the guide wire using the cannulated screwdriver shaft.



**6**  
CHECK: Neither the thread head nor the screw tip should protrude from the bone.

**7**  
Remove the K-Wire.



Order online at:  
**veterinary.shop**



ACADEMY

LEARN FROM THE BEST  
**WORKSHOPS**

See Workshops und Online Courses at our Academy Page.

**academy.leibinger.vet**

**NEW**

### LeiCOM Combi Set

All sizes of our Titanium Cannulated Compression Bone Screws - 2.4/3.1 Micro, 3.0/3.9 Mini, 4.0/5.0 Medi and 5.0/6.0 Maxi - plus essential instruments **in one compact set**.

### LeiCOM Cannulated Compression Screws Combi Set - 2.4 - 6.0 Micro to Maxi



Contains:

- 1 LEICOM Compression Screws Set Tray with Lid
- 1 of each LEICOM Compression Screws (Micro 2.4/3.1, 8-30mm // Mini 3.0/3.9, 10-40mm // Medi 4.0/5.0, 14-60mm // Maxi 5.0/6.0, 20-60mm // 61 total)
- 1 Screwdriver Handle
- 1 of each Screwdriver Shaft T6 & T8, cannulated (2.4 & 3.0mm)
- 1 of each Screwdriver Shaft T10 & T15, cannulated (4.0 & 5.0mm)
- 1 of each Screw Head countersink, cannulated (2.4 & 3.0mm)
- 1 of each Screw Head countersink, cannulated (4.0 & 5.0mm)
- 1 of each Drill Bit (Ø 1.8mm, 2.3mm, 2.7mm & 3.8mm)
- 1 Screw Depth Gauge
- K-Wires (Ø 0.9mm x 150mm, Ø 1.5mm x 150mm)

**244-2460-00**


Tray without contents

**244-2460-10**

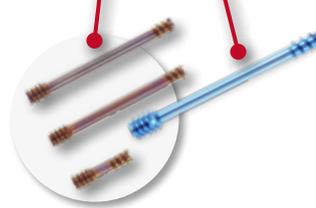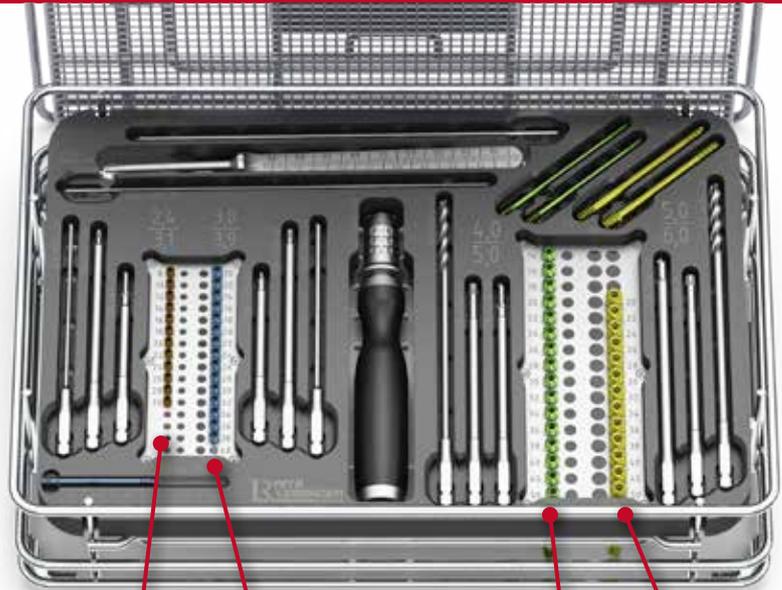

**2.4/3.1 LeiCOM Micro**  
8mm - 30mm in length

**3.0/3.9 LeiCOM Mini**  
10mm - 40mm in length



**4.0/5.0 LeiCOM Medi**  
14mm - 60mm in length

**5.0/6.0 LeiCOM Maxi**  
20mm - 60mm in length



### FEATURED CASE

#### SCAPULA FRACTURE TREATMENT WITH A RAPID PATELLA LUXATION PLATE & LEICOM COMPRESSION SCREW

Read about an interesting case of a 9-year-old Old English Bulldog with a complex multifragment fracture of the scapula.

This case was shared with us courtesy of Dr. Johannes Frahm, Dr. Dominik Wilke, and the wonderful team of Wasbek Veterinary Clinic in Germany.

Read the full story at:  
[www.leibinger.vet/blog](http://www.leibinger.vet/blog)

**LeiCOM Cannulated  
Compression Screws Set -  
2.4 / 3.1 Micro & 3.0 / 3.9 Mini**

Contains:

- 1 LEICOM Compression Screws Set Tray with Lid
- 1 of each LEICOM Compression Screws  
(Micro 2.4, 8-14mm & 24-30mm // Mini 3.0,  
10-18mm & 32-40mm // 18 total)
- 2 of each LEICOM Compression Screws  
(Micro 2.4, 16-22 // Mini 3.0, 20-30mm // 20 total)
- 1 Screwdriver Handle
- 1 of each Screwdriver Shaft T6 & T8,  
cannulated (2.4 & 3.0mm)
- 1 of each Screw Head countersink,  
cannulated (2.4 & 3.0mm)
- 1 of each Drill Bit (Ø 1.8mm & 2.3mm)
- 5 K-Wires (Ø 0.9mm x 150mm)



**244-2439-00**

Tray without contents

**244-2439-10**

**2.4 LeiCOM Micro Compression Screw**

Cannulated Bone Screw 2.4 x 3.1 mm, Titanium  
LeiStar, self-tapping, self-drilling

**3.0 LeiCOM Mini Compression Screw**

Cannulated Bone Screw 3.0 x 3.9 mm, Titanium  
LeiStar, self-tapping, self-drilling



Length (mm)	Product Code
08	244-2431-08
10	244-2431-10
12	244-2431-12
14	244-2431-14
16	244-2431-16
18	244-2431-18
20	244-2431-20
22	244-2431-22
24	244-2431-24
26	244-2431-26
28	244-2431-28
30	244-2431-30

Length (mm)	Product Code
10	244-3039-10
12	244-3039-12
14	244-3039-14
16	244-3039-16
18	244-3039-18
20	244-3039-20
22	244-3039-22
24	244-3039-24
26	244-3039-26
28	244-3039-28
30	244-3039-30
32	244-3039-32
34	244-3039-34
36	244-3039-36
38	244-3039-38
40	244-3039-40

Compression Bone Screws Set - Medi/Maxi

Compression Bone Screws 4.0 - 6.0

**LeiCOM Cannulated  
Compression Screws Set -  
4.0 / 5.0 Medi & 5.0 / 6.0 Maxi**

Contains:

- 1 LEICOM Compression Screws Set Tray with Lid
- 1 of each LEICOM Compression Screws (Medi 4.0, 14-24mm & 38-60mm // Maxi 5.0, 20-28mm & 40-60mm // 22 total)
- 2 of each LEICOM Compression Screws (Medi 4.0, 26-36// Maxi 5.0, 30-38mm // 22 total)
- 1 Screwdriver Handle
- 1 of each Screwdriver Shaft T10 & T15, cannulated (4.0 & 5.0mm)
- 1 of each Screw Head countersink, cannulated (4.0 & 5.0mm)
- 1 of each Drill Bit (Ø 2.7mm & 3.8mm)
- 5 K-Wires (Ø 1.5mm x 150mm)



**244-4060-00**

Tray without contents

**244-4060-10**

**4.0 LeiCOM Medi Compression Screw**

Cannulated Bone Screw 4.0 x 5.0 mm, Titanium LeiStar, self-tapping, self-drilling

**5.0 LeiCOM Maxi Compression Screw**

Cannulated Bone Screw 5.0 x 6.0 mm, Titanium LeiStar, self-tapping, self-drilling



Length (mm)	Product Code
14	244-4050-14
16	244-4050-16
18	244-4050-18
20	244-4050-20
22	244-4050-22
24	244-4050-24
26	244-4050-26
28	244-4050-28
30	244-4050-30
32	244-4050-32
34	244-4050-34
36	244-4050-36
38	244-4050-38
40	244-4050-40
45	244-4050-45
50	244-4050-50
55	244-4050-55
60	244-4050-60

Length (mm)	Product Code
20	244-5060-20
22	244-5060-22
24	244-5060-24
26	244-5060-26
28	244-5060-28
30	244-5060-30
32	244-5060-32
34	244-5060-34
36	244-5060-36
38	244-5060-38
40	244-5060-40
45	244-5060-45
50	244-5060-50
55	244-5060-55
60	244-5060-60



Screw Depth Gauge, cannulated

Screwdriver Shaft, cannulated

**Screwdriver Handle**

Silicone, AO-Connection  
sterilizable up to 134°C / 273°F



Product Code	Description
247-0105-00	standard, straight, black

**Screw Depth Gauge, cannulated**

for K-Wires up to Ø 1.6, cannulated 150



164-1600-00



**K-Wire, Single Trocar**

Length: 150 mm, round end



Product Code	Ø x Length (mm)
144-1009-15	0.9 x 150
144-1015-15	1.5 x 150

**Screwdriver Shaft LeiStar, cannulated**

For LeiCOM, AO connection



Product Code	Description
128-2431-06	2.4 mm, 90mm, cannulated, T6 for 2.4 / 3.1 mm screws
128-3039-08	3.0 mm, 90mm, cannulated, T8 for 3.0 / 3.9 mm screws
128-4050-10	4.0 mm, 90mm, cannulated, T10 for 4.0 / 5.0 mm screws
128-5060-15	5.0 mm, 90mm, cannulated, T15 for 5.0 / 6.0 mm screws

Screw Head Countersink, cannulated

Drill Bits, cannulated

**Screw Head Countersink LeiStar, cannulated**  
For LeiCOM, AO connection



Product Code	Description
128-2431-31	2.4 mm, 70mm, cannulated, for 2.4 / 3.1 mm screws
128-3039-39	3.0 mm, 70mm, cannulated, for 3.0 / 3.9 mm screws
128-4050-50	4.0 mm, 90mm, cannulated, for 4.0 / 5.0 mm screws
128-5060-60	5.0 mm, 100mm, cannulated, for 5.0 / 6.0 mm screws



**Drill Bits, cannulated**

Length 95mm, Cannulation Ø 1.1 mm, AO Connection



Product Code	Ø (mm)
148-0084-18	1.8
148-0084-23	2.3

**Drill Bits, cannulated**

Length 125mm, Cannulation Ø 1.6 mm, AO Connection



Product Code	Ø (mm)
148-0084-27	2.7
148-0084-38	3.8



# Suture Anchor Screws

## High-Strength Titanium Suture Anchors

The RITA LEIBINGER Suture Anchor Screws are made of high-grade Titanium, making them very durable but lightweight. This material also allows for the design of thinner and smaller-sized anchors without compromising strength.

## Titanium: Best Biocompatibility

Made from a unique Titanium alloy, our suture/bone anchors are highly biocompatible and has low temperature sensitiveness. The high-strength material and construct provides fixation strength and stability, which promotes healing of the soft tissue.

## Easy to use

The self-tapping design of our threaded suture anchors makes them easy to use and position, therefore shortening surgery time. Simply drill in the bone anchor using a Jacob's Chuck and snap the rod off.

## Secure and stable fixation

The stable construct ensures a secure fixation of the suture anchor, thereby maintaining the position of the anchor without loosening and providing optimal conditions for rapid and uninterrupted healing of the soft tissue.

## Quality that is affordable

The Suture Anchor Screws from RITA LEIBINGER are manufactured at our own plant in Germany. We can therefore offer you high-quality products at very affordable prices.

**BEST QUALITY**  
**MADE IN GERMANY**



Special Thanks to  
Dr. Hugo Schmökel

# SUTURE ANCHORS

**R** RITA  
LEIBINGER  
MEDICAL

Suture Anchor

Crimp Tubes

2.0 Suture Anchor

Titanium

144-8888-20



Total Length	45 mm
Thread Length	7 mm
Hole Ø	0.65 mm



2.4 Suture Anchor

Titanium

144-8888-24



Total Length	45 mm
Thread Length	7 mm
Hole Ø	0.85 mm

2.7 Suture Anchor

Titanium

144-8888-27



Total Length	45 mm
Thread Length	9 mm
Hole Ø	1.5 mm



3.5 Suture Anchor

Titanium

144-8888-35



Total Length	45 mm
Thread Length	11.5 mm
Hole Ø	2.0 mm

Crimp Tubes

Stainless Steel, Sold in 12-pc packs, non-sterile



Product Code	Ø (mm)	Description
143-0001-10	10	Crimp Tube for 50lb lines
143-0001-12	12	Crimp Tube for 80lb + 100 lb lines
143-0001-14	14	Crimp Tube for nylon lines over 100lb

## Sutures

## Tensioning Device

## Crimper

**CCL Cruciate Surgical Sutures + Crimp**

Nylon cruciate surgical sutures with needle and crimps



Product Code	Description	Needle	Crimps
143-0008-50	50lb CCL nylon line (500mm) on swaged-on very small fabella needle (30mm) plus 1x10mm crimp, sterile	Very Small 30 mm	1 x 10mm crimp
143-0010-50	50lb double CCL nylon line (500mm x 2 as loop) on swaged-on very small fabella needle (30mm) plus 2x10mm crimps, sterile	Very Small 30 mm	2 x 10mm crimps
143-0008-80	80lb CCL nylon line (800mm) on swaged-on small fabella needle (45mm) plus 1x12mm crimp, sterile	Small 45 mm	1 x 12 mm crimp
143-0010-80	80lb double CCL nylon line (800mm x 2 as loop) on swaged-on small fabella needle (45mm) plus 2x12mm crimps, sterile	Small 45 mm	2 x 12mm crimps
143-0008-100	100lb CCL nylon line (800mm) on swaged-on medium fabella needle (62mm) plus 1x12mm crimp, sterile	Medium 62 mm	1 x 12mm crimp
143-0010-100	100lb double CCL nylon line (800mm x 2 as loop) on swaged-on medium fabella needle (62mm) plus 2x12mm crimps, sterile	Medium 62 mm	2 x 12mm crimps

**Crimper**

Orthofiber Crimping Device TC, 23 cm

**129-0051-23**

**Universal Tensioning Device**

17 cm


**24-4310-17**


# C-LOX Cervical Intervertebral Fusion Implant



## Versatility and Stability

The cages come in different sizes to fit different breeds and spinal segments. Developed to combine the benefits of an intervertebral spacer, rigid titanium plate, and locking screw fixation, the C-LOX Cages not only preserve the natural anatomic profile of the spine, but also provide great stability and convenience in placement and fixation.

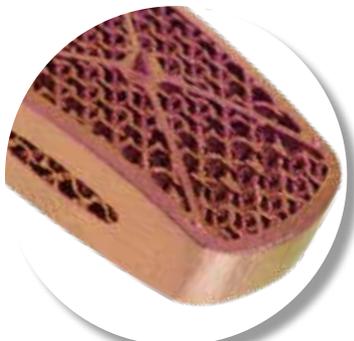

## Improved Osseointegration

The dodecahedron construct of the cage provides a larger surface area for bone growth, which improves osseointegration and cell attachment, therefore promoting bone growth and reducing implant failure rates.



## Exceptional Biocompatibility & Strength

With minimal adverse reactions or rejections, Titanium reduces the risk of infection and inflammation. Its hypoallergenic properties make it a safe choice, reducing the likelihood of allergic responses. The unique Titanium Alloy also makes our implants and screws very durable but lightweight.




## LeiStar Screws

The C-LOX Locking screws have LeiStar screwheads, which allows for best tightening torque. Additionally, the screws provide a self-holding feature when used with a RITA LEIBINGER screwdriver shaft, keeping the screws securely on the driver.

# **C-LOX**®

*Makes the lame walk again.*

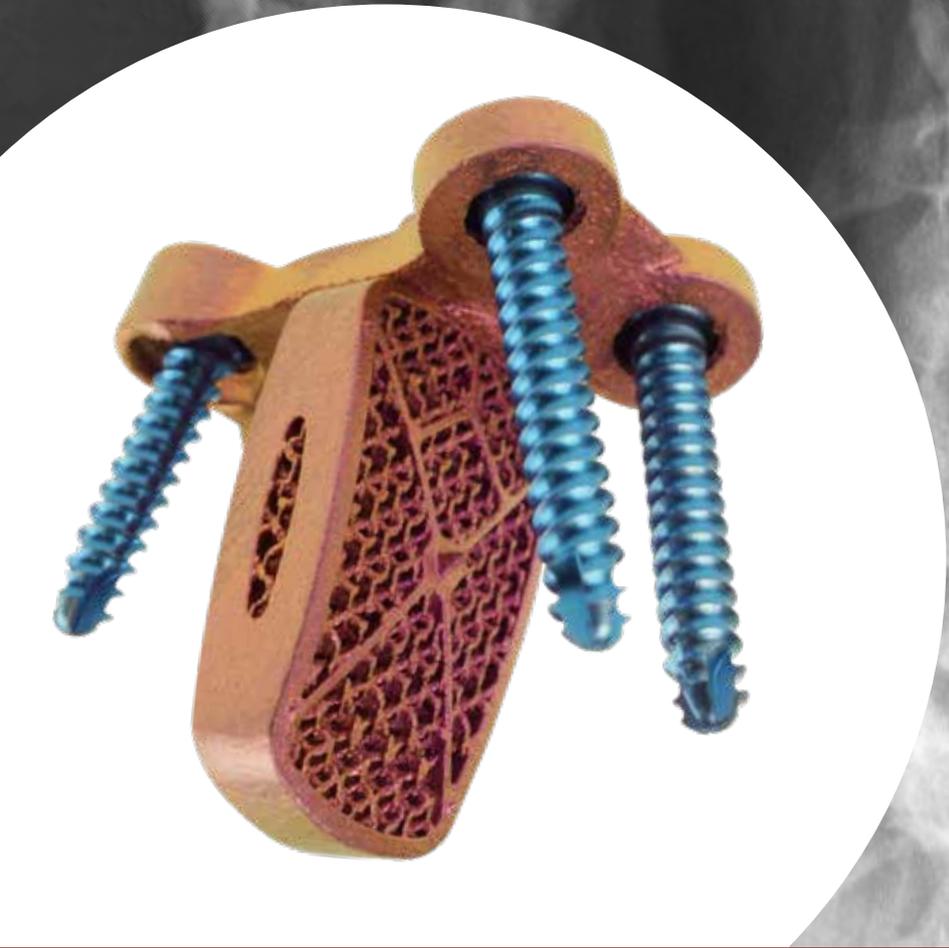

Special Thanks to  
Prof. Björn Meij



## **C-LOX SPINAL, locking**

**R** **RITA**  
**LEIBINGER**  
MEDICAL

## C-LOX

### Surgical Protocol

#### Surgical application of a new anchored intervertebral spacer (C-LOX) for the treatment of Canine Cervical Spondylomyelopathy (Wobbler Syndrome)

Authors: Dr. Günter Schwarz & Prof. Dr. Franck Forterre

NOTE: Preoperative radiographs are used to make preliminary selection of spacer and screw sizes. It is advisable but not indispensable to use fluoroscopy while performing the distraction-fusion technique with the C-Lox Cage. Fluoroscopy will provide accurate intraoperative assessment of correct implant and screw size, and of the depth and location of spacer and screw placement.



**(1)** Place the dog in dorsal recumbency with a fulcrum underneath to support the neck. Avoid overextension. A standard approach to the ventral cervical spine is performed.



**(2)** The affected disc space is identified and exposed, and a window is cut out of the ventral annulus fibrosus using a beaver blade. The width of this window should be minimally larger than the width of the selected spacer. The vertebral endplates delimit the cranial and caudal borders of the opening. Care must be taken not to penetrate the dorsal part of the annulus during discectomy.



**(3)** In order to attach the C-LOX Distractor, vertically oriented 2.5 mm holes are drilled into each of the adjacent vertebrae. These holes must be exactly on the midline and should be located in the caudal half of the cranial and in the cranial half of the caudal vertebrae. Penetration depth should at least be 2/3 of the vertebral body depth in order to avoid tilting when distracting the vertebrae. The crista ventralis marks the median plane of the vertebrae but makes it easy to slide off the midline. Preoperative measurements and fluoroscopy will aid in taking care not to enter the spinal canal.



Insert the C-LOX Distractor into the predrilled holes and open its jaws to widen the intervertebral disc space.



**(4)** The C-LOX Spinal Disc Broaching Curette is used to carefully remove all remnants of the nucleus pulposus. The dorsal part of the annulus fibrosus can be felt as a more dense structure and should be preserved. The exposed

end plates are freed from as much connective tissue as possible, but subchondral bone must be fully preserved.

If a considerable amount of nucleus pulposus material is located within the spinal canal, this can be attempted to remove with

the help of fine curettes or delicate arthroscopic biopsy forceps.

**(5)** The suitable size for the C-Lox implant can be estimated pre-operatively on diagnostic imaging. Attach the C-LOX Implantation Placement Rod to the suitable C-LOX Template and insert it in the intervertebral disc space. Ensure the correct fit. Here again, vertical beam fluoroscopy can be very helpful. If insertion requires energetic forcing or seems to achieve only slight distraction, a slimmer or thicker template should be used.



**(6)** After establishing optimal fit, the Template is replaced by the corresponding C-LOX Cage. Spikes on the cranial and caudal side will ensure a secure seating of the implant, but can make insertion slightly more difficult compared to the C-Lox Template of the same size. Press the cage firmly down into place.



**(7)** After proper seating of the C-Lox Cage, the C-Lox Distractor can be removed and the Implantation Placement Rod is removed from the cage. The cage will be secured with locking screws.



**(8)** Select the drill guide according to the screw length intended to use. Attach the Drill Guide to the Implant and use the dedicated 2.0mm drill bit to drill the hole for the Locking Cortical Screw. This drill bit forms a unit with the Drill Guide and will create the hole in the vertebral body to guide the self tapping screw. Screw Lengths are selected pre-operatively from measurements on the preoperative radiographs in precise latero-lateral projection. The four Locking Cortical Screw are inserted using the LeiStar C-Lox Screwdriver. The screws must be well anchored within the vertebral body and must not penetrate the vertebral end plates or the spinal canal. Again, fluoroscopy can be very helpful in



achieving optimal screw placement.

**(9)** Cancellous bone or bone substitutes can be apposed to the ventral surface of the treated disc space.

Close the soft tissues in a routine manner.

## C-LOX Set

Contains:

- Sterilization Tray with Lid
- 1 of each Spinal Cage
- 1 of each Seizing Cage
- 2 Placement Rods
- Spinal Curette
- Screwdriver Shaft
- Screwdriver Handle Silicone
- 1 of each Locking Drill Guide
- 2 Drills (2.0/2.5mm)
- 5 of each Screw (10, 12, 14, 16, 18, 20mm)  
(30 pcs. total)

**134-0100-01**

Tray without contents

**134-0500-01**



## C-LOX Cervical Intervertebral Fusion Implant

C-LOX was developed  
by RITA LEIBINGER in cooperation with  
**Professor Dr. Franck Forterre**,  
Bern University (Switzerland).

For more details please visit:

**spinal.leibinger.vet**



**C-LOX**




14 x 4 x 8 mm

14 x 6 x 8 mm

16 x 4 x 8 mm

16 x 6 x 8 mm

16 x 5 x 10 mm

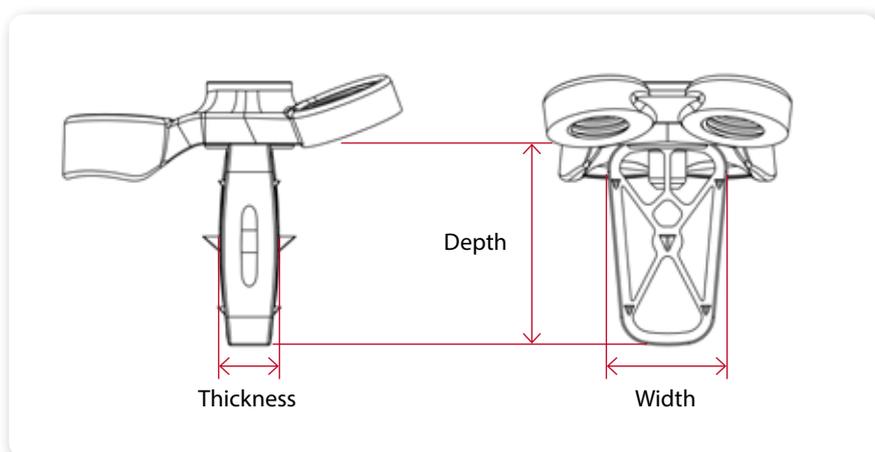

**C-LOX Cages**

Titanium

Product Code	Dimensions		
	Depth	Thickness	Width
134-0144-08	14 mm	4 mm	8 mm
134-0146-08	14 mm	6 mm	8 mm
134-0164-08	16 mm	4 mm	8 mm
134-0165-10	16 mm	5 mm	10 mm
134-0166-08	16 mm	6 mm	8 mm
134-0167-10	16 mm	7 mm	10 mm
134-0185-10	18 mm	5 mm	10 mm
134-0187-10	18 mm	7 mm	10 mm
134-0206-12	20 mm	6 mm	12 mm
134-0208-12	20 mm	8 mm	12 mm



16 x 7 x 10 mm

18 x 5 x 10 mm

18 x 7 x 10 mm

20 x 6 x 12 mm

20 x 8 x 12 mm

### C-LOX Templates

Titanium




Product Code	Dimensions		
	Depth	Thickness	Width
134-9144-08	14 mm	4 mm	8 mm
134-9146-08	14 mm	6 mm	8 mm
134-9164-08	16 mm	4 mm	8 mm
134-9165-10	16 mm	5 mm	10 mm
134-9166-08	16 mm	6 mm	8 mm
134-9167-10	16 mm	7 mm	10 mm
134-9185-10	18 mm	5 mm	10 mm
134-9187-10	18 mm	7 mm	10 mm
134-9206-12	20 mm	6 mm	12 mm
134-9208-12	20 mm	8 mm	12 mm



### Locking Selfdrilling Cortical Screw

Titanium, LeiStar Head, self-tapping with three flute cutting edge



Product Code	Total Length	Thread Length
245-427-08	10 mm	8 mm
245-427-10	12 mm	10 mm
245-427-12	14 mm	12 mm
245-427-14	16 mm	14 mm
245-427-16	18 mm	16 mm
245-427-18	20 mm	18 mm
245-427-20	22 mm	20 mm

### Screwdriver Handle

Silicone, AO-Connection  
sterilizable up to 134°C / 273°F

**247-0102-00**



### Torque Limiting Screwdriver Handle

Torque 3 Nm  
Silicone, AO, sterilizable up to 134°C / 273°F

**247-0104-00**



### C-LOX Screwdriver Shaft 2.7

LeiStar, 135mm length, AO

**134-0800-27**



Instruments, C-LOX

C-LOX Utilities

C-LOX Locking Drill Guides

Stainless Steel  
for 2.0mm drills, for 2.7mm screws



Product Code	Description
164-0027-10	10 mm working end
164-0027-12	12 mm working end
164-0027-14	14 mm working end

Product Code	Description
164-0027-16	16 mm working end
164-0027-18	18 mm working end
164-0027-20	20 mm working end

C-LOX Drill

Product Code	Ø (mm)	Connection
148-0081-20	2.0	AO QC
148-0081-25	2.5	AO QC



C-LOX Spinal Curette

22cm

134-0700-22



C-LOX Implant Placement Rod

22 cm

134-0750-22



C-LOX Distractor

Product Code	Description
134-0750-16	50mm deep, 160mm length, 90° curved
134-0750-20	50mm deep, 200mm length, 90° curved



# LeiLa Bone Substitutes




## Easy Application

**LeiLa REDy Hydroxyapatite Paste** comes in a ready-to-use syringe, making it easy to apply in any situation. Application of our **LeiLa Bone Matter** Bone Graft Granules is straightforward: first, transfer the contents of the ampoule into a suitable container. Next, mix the LeiLa Bone Matter with a small amount of the patient's blood. Once combined, press the mixture into the bone defect. Finally, close the wound. It's as simple as that!



## 0% Risk of Disease Transmission

Made of 100% synthetic biocompatible materials and manufactured under sterile conditions, LeiLa Bone Substitutes can spare patients the trauma of autograft harvesting and provides a fully synthetic alternative to animal cadaver bone grafts, therefore carrying no risk of contamination and disease transmission.

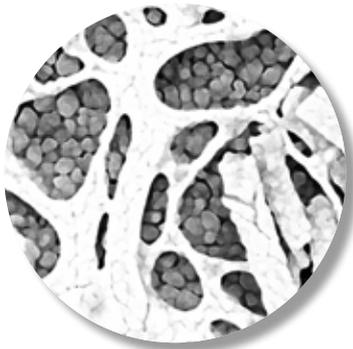

## Excellent Bioactivity, Osteoconductivity, & Resorbability

Made of biocompatible material, our bone substitutes form a strong bond with the surrounding bone tissue, facilitating the formation of a stable and long-lasting implant that can effectively promote healing and regeneration. Its high resorbability allows it to be efficiently replaced by new bone tissues, resulting in complete and natural bone regeneration.



## Multiple Applications

The LeiLa Bone Substitutes can be used in many different cases including filling and supporting the ingrowth of adjacent viable bone in bone defects that do not compromise the structural stability of the bone. They are also ideal for filling bone defects in cases of fractures and following the resection of benign tumors or cysts. They are perfect for filling and supporting the regeneration of bone at autograft harvest sites, and they are also ideal for addressing defects of the alveolar ridge or wall, including extraction sockets. Additionally, LeiLa Bone Substitutes provide excellent support for periodontal bone regeneration.




## Radiopaque

Visible on x-rays and other imaging studies, making it easier for veterinary surgeons to accurately monitor the healing process, until the bone substitute is totally resorbed.



**Leila**  
SERIES  
RITA LEIBINGER LABS

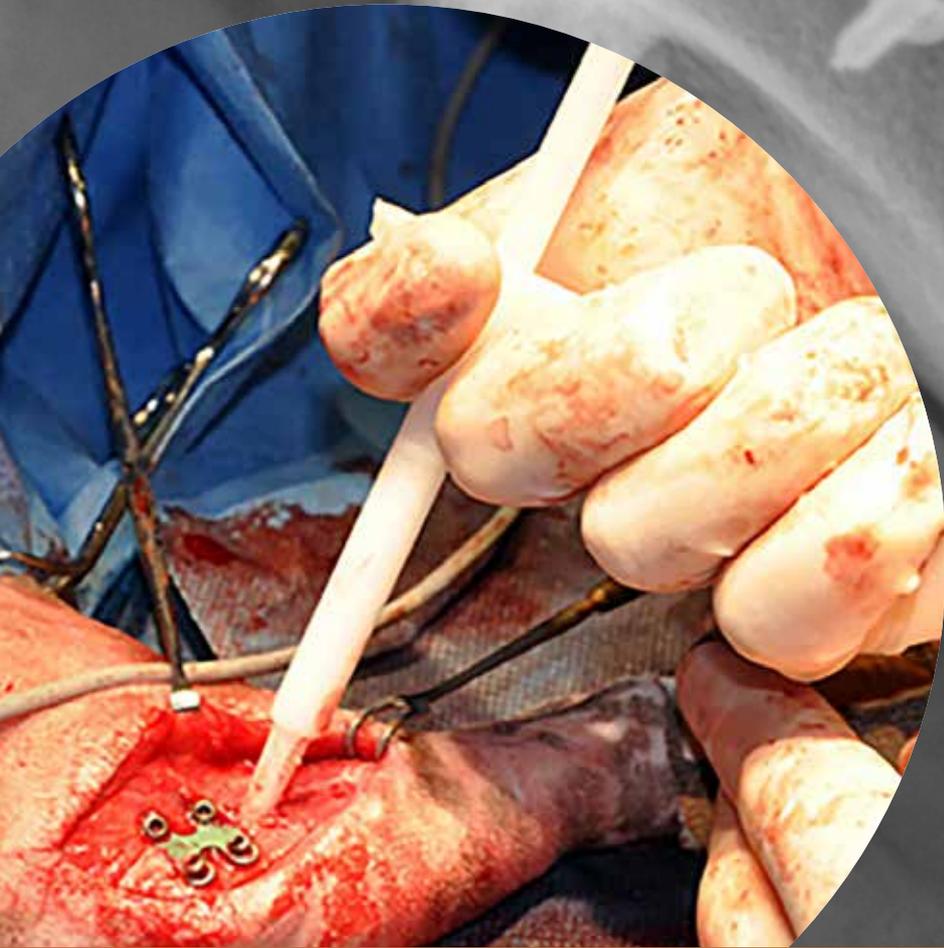

Special Thanks to  
Siegfried Wilhelm

**Leila BONE MATTER**




**RITA**  
**LEIBINGER**  
MEDICAL

**LeiLa REDY Hydroxyapatite Paste**

1 x 2.5 g syringe, sterile

synthetic resorbable Bone Substitute, Hydroxyapatite

132-9025-00

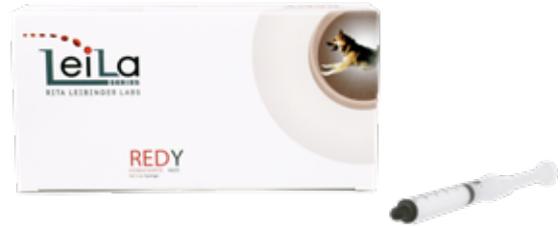

**LeiLa REDY ONEg Hydroxyapatite Paste**

3 x 1 g syringe, sterile

synthetic resorbable Bone Substitute, Hydroxyapatite

140-2011-00



**SYNTHETIC CERAMIC NANO-HYDROXYAPATITE PASTE**

**REDY Hydroxyapatite paste** is a synthetic (Alloplast) ceramic, composed by a water based nano-hydroxyapatite paste.

It is resorbed and replaced by natural bone as bone healing process occurs and the paste can be molded to follow the natural contours of the bone.

**REDY Hydroxyapatite paste** can, in many cases, spare the patient the trauma of autograft harvesting and provides an alternative to animal cadaver bone.

**LeiLa Bone Matter**

99,9% tricalcium phosphate Economic, 5x1 gram-package, sterile

140-1011-00



**POROUS SYNTHETIC CERAMIC BONE GRAFT**


**Bone Matter** is a fully synthetic bone graft biomaterial, composed of pure beta-tricalcium phosphate ( $\beta$ -TCP).

**Bone Matter** features a multidirectional interconnected porosity that guides the three-dimensional bone regeneration.

As bone healing occurs, **Bone Matter** is resorbed and replaced by new bone.

**Why choose LeiLa Bone Matter and LeiLa REDY?**

- Radiopaque allowing the monitorization of the graft osteointegration
- Quickly resorbed and replaced by new bone
- Provides an alternative to autologous bone graft harvesting, and is an alternative to animal cadaver bone
- Do not contain animal or human tissues or derivatives
- Intended to be used as a filling material for bone voids or defects which are not intrinsic to the stability of the bone

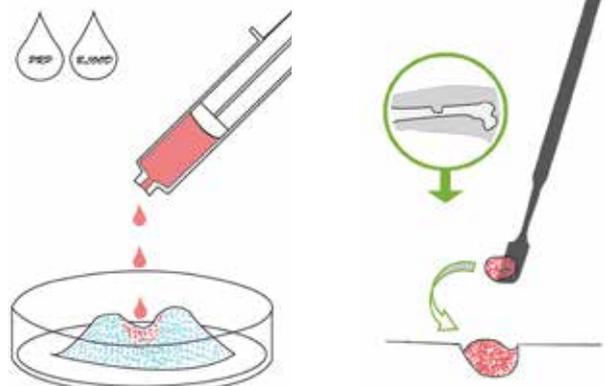

Find more product information online.



Special Thanks to  
Dr. Hugo Schmökel

# Small Animal **ARTHROSCOPY**

## ABOUT ARTHROSCOPY

**Prof. Dr. Bernadette Van Ryssen***DVM, PhD, Dipl. ECVSMR*Department of Medical Imaging &  
Small Animal Orthopaedics  
Faculty of Veterinary Medicine  
GHENT UNIVERSITY

“

In the last few decades, arthroscopy in small animals has known a rapid expansion because of some important advantages. This minimally invasive technique allows a wide and detailed inspection of the intra-articular structures and their pathologic changes because of the enlargement by the arthroscope and camera. Fibrillation and superficial erosions of cartilage, fibers of (partially) ruptured ligaments, and the structure of synovial villi are details that can be evaluated during arthroscopy. These possibilities allow an accurate diagnosis and a better understanding of the intra-articular anatomy and pathology. Arthroscopy can be used to demonstrate discrete or early lesions without radiographic evidence. It allows a second look in joints that have been treated unsuccessfully via arthrotomy or arthroscopy.

Several lesions can be treated via arthroscopy. In case of bilateral lesions, treatment of both joints can be performed during one anesthesia. Because of the limited surgical trauma, the postoperative care and risk for complications are minimal.

A prerequisite for successful arthroscopic interventions is good quality equipment to clearly visualize the intra-articular structures. It is also important to work with the correct instruments: they should be small yet strong and have an adapted shape.

Finally, training and exercise is needed before sufficient experience is reached to apply arthroscopy in the small sized joints and to adapt a different way of surgical handling.


*Original English text from Prof. Dr. Van Ryssen*

”

**arthroscopy.leibinger.vet**

## Van Ryssen Arthroscopy Set

111-0016-00

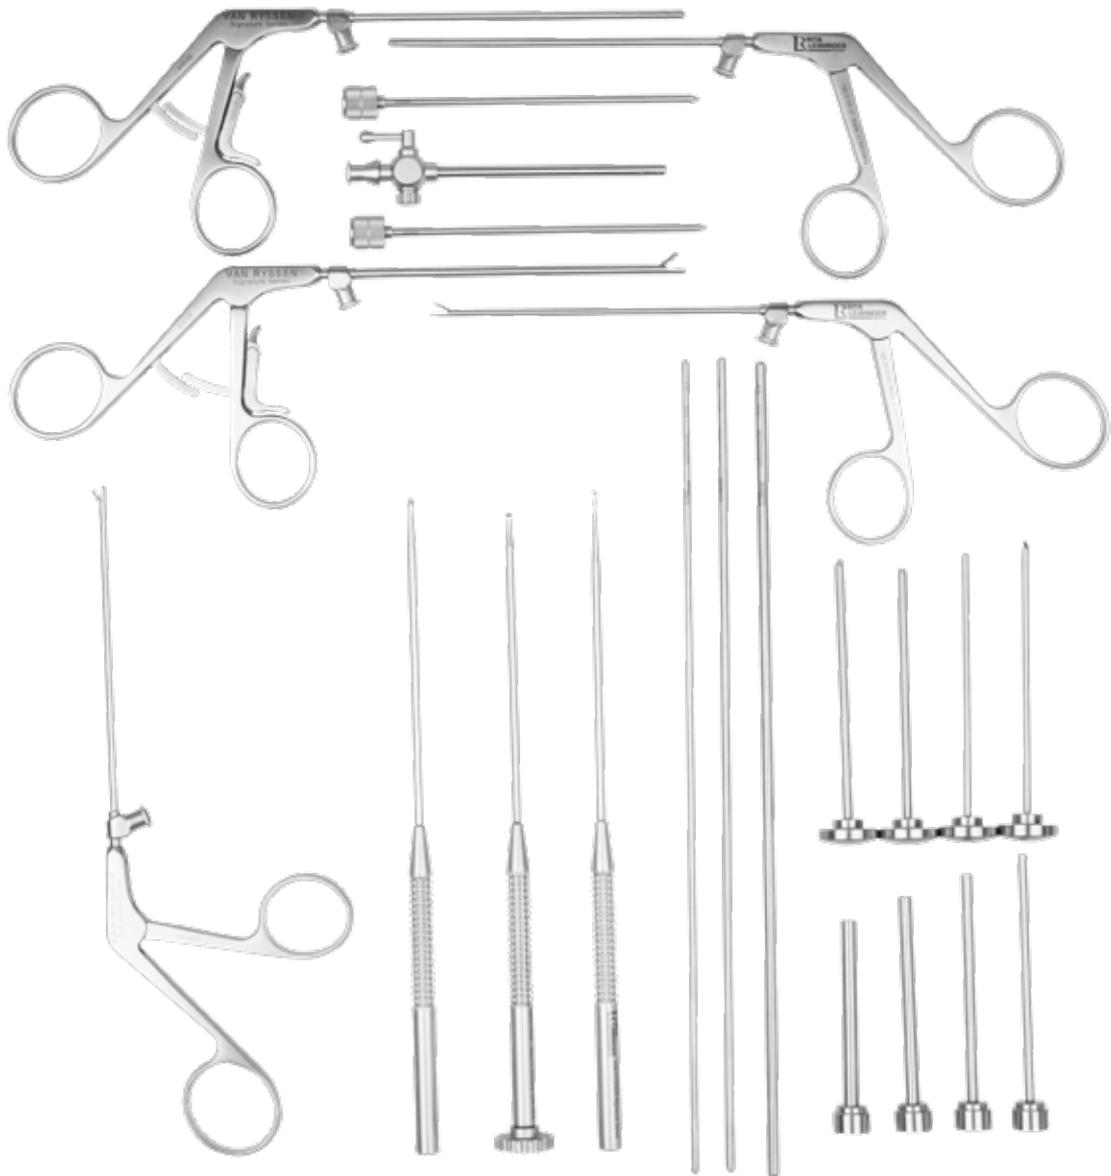


Product Code	Description
165-0100-21	Marking Rod 2.1 mm, working length 250 mm
165-0100-27	Marking Rod 2.7 mm, working length 250 mm
165-0100-34	Marking Rod 3.4 mm, working length 250 mm
162-0112-02	Grasping Forcep Alligator, $\varnothing$ 2.0 mm, with fine serration, with flush port, working length 110 mm
162-0146-02	Biopsy Spoon, with flush port, 110 mm working length, sharp, $\varnothing$ 2.0 mm
162-0169-30	Grasping Forcep, with spoon, 1x2 teeth, cross serrated, $\varnothing$ 3.0 mm, with flush port, working length 110 mm
162-0182-27	Hook Scissors, $\varnothing$ 2.7 mm, with flush port, working length 110 mm
162-0197-27	Biopsy Spoon, sharp, $\varnothing$ 2.7, cross serrated, with flush port, working length 110 mm, with ratchet
165-0110-15	Hook Probe, 1.5 mm
165-0110-23	Ball Head Burr, 2.3 mm
165-0120-15	Spoon Curette, small model, 1.5 mm
165-0150-32	Rinse Cannula, complete with Trocar/Obturator, 3.2 mm, with Stopcock
165-0100-00	4 Sheaths, 2.2 / 2.8 / 3.5 / 4.2 mm, 2 Trocar pyramid tip, 2 Obturators round



## Van Ryssen Series

*Intelligent design in collaboration with Prof. Dr. Bernadette van Ryssen*

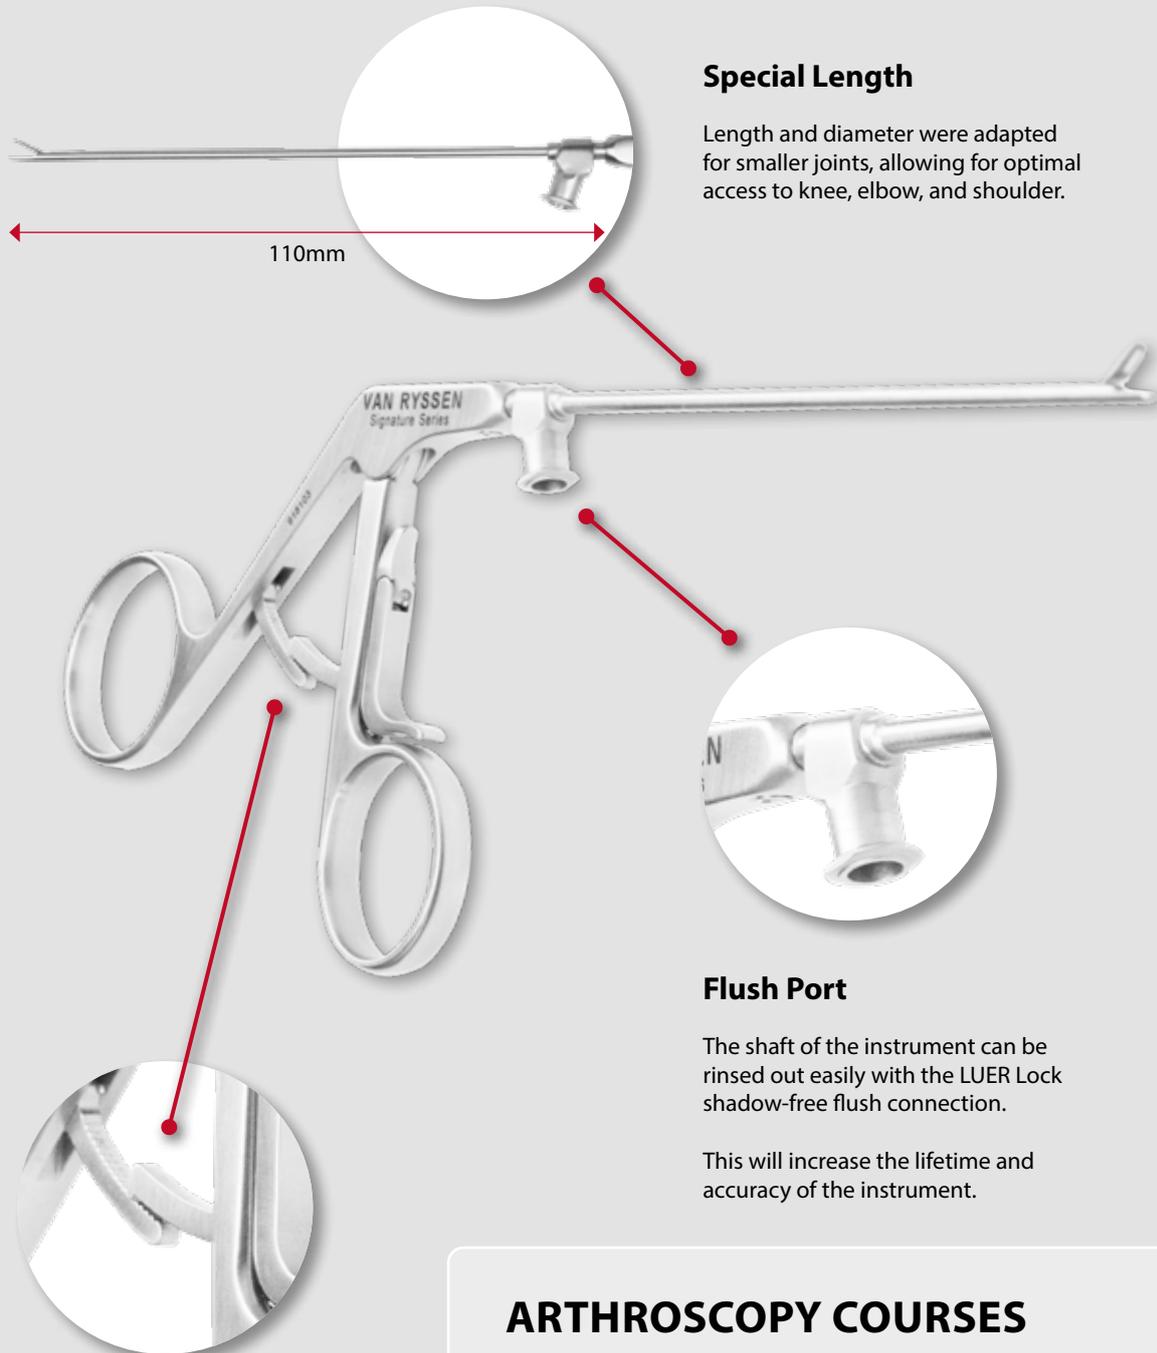

### Special Length

Length and diameter were adapted for smaller joints, allowing for optimal access to knee, elbow, and shoulder.

110mm

### Flush Port

The shaft of the instrument can be rinsed out easily with the LUER Lock shadow-free flush connection.

This will increase the lifetime and accuracy of the instrument.

### Special Ratchet

Innovative ratchet mechanism for a quick switch between ratchet and ratchet-free working.

## ARTHROSCOPY COURSES

Learn Arthroscopy with Prof. Dr. Bernadette van Ryssen and other experts.

Explore available courses at our Academy page:

[academy.leibinger.vet](https://academy.leibinger.vet)



ACADEMY

Grasping Forcep Alligator

Hook Scissors

Biopsy Spoon Forceps

**Grasping Forcep Alligator**

Fine serration, with flush port  
2.0 mm, 110 mm Shaft

**162-0112-02**



**Hook Scissors**

Sharp, with flush port  
2.7 mm, 110 mm Shaft

**162-0182-27**



**Biopsy Spoon Forceps**

Sharp, with flush port  
2.0 mm, 110 mm Shaft

**162-0146-02**



**Biopsy Grasping Forceps**

With spoon, 1x2 teeth, with ratchet, flush port  
3.0 mm, 110 mm Shaft

**162-0169-30**



**Biopsy Spoon Forceps**


Cross serrated, with ratchet, flush port  
2.7 mm, 105 mm Shaft

**162-0197-27**



## Van Ryssen Signature Series

*RITA LEIBINGER MEDICAL proudly presents a new ergonomic grip design.*

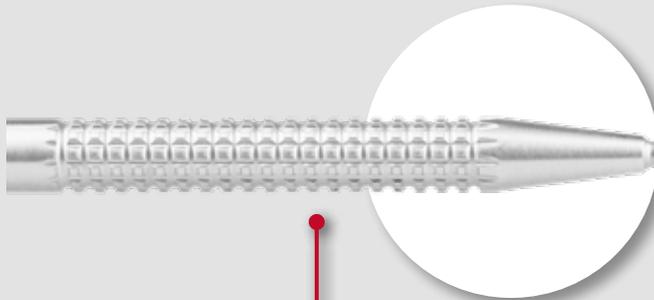

### New Grip Design

The new anti-slip grip design is ergonomically well balanced and provides an easy control of the working end. This results in a fatigue-free surgery.



### Mushroom Handle for Ball Head Burr

The redesign of the mushroom handle, combined with a new grip design, allows the ball head burr to be used with greater accuracy and efficiency, saving time.



### Small Working Ends

The size of the working ends has been reduced, enabling precise fine work, particularly in small joints.

Hook Probe

Ball Head Burr

Knives

Hook Probe

Product Code	Description
165-0110-10	1.0 mm
165-0110-15	1.5 mm



Ball Head Burr

2.3 mm

165-0110-23



Spoon Curette

Product Code	Description
165-0120-15	1.5 mm
165-0120-30	2.7 mm



Banana Knife

2.5x12 mm

165-0130-00



Hook Knife

2.2 mm

165-0130-22



Elevator

Penfield Style, small  
2.5 mm

165-0140-00



Curette

2.7 mm with hole

165-0120-28



Meniscus Knife

2.5 mm

165-0130-25



Arthroscopy Standard Instruments

**Standard Instrument, 2.0mm**

Product Code	Description
162-0150-11	Hook Scissors, Ø 2.0mm shaft, 11cm long



**Standard Instrument, 3.4mm**

Product Code	Description
162-0190-34	Hook Punch Forceps, 3.4mm, straight, with scoop, 15cm long



**Standard Instrument with knurled handle (Ø 4.0mm)**

*"knurled" handle*



**Hook Knife**  
fine  
160-2401-00



**Meniscotome**  
5.0 mm  
160-2402-00



**Meniscotome**  
7.0mm  
160-2413-00



**Smillie-Meniscotome**  
3mm  
160-2408-00



**Meniscus Rasp**  
fine  
160-2420-00



**Meniscus Rasp**  
coarse  
160-2421-00



**ATTENTION: only while stocks last.**

Arthroscopes

Arthroscopy Trocar Set

**Arthroscopes**

**Optics**

Autoclavable up to 134°C / 273°F



	Product Code	Description
●	162-0016-30	2.0 mm / 110 mm / 30° Optic
▲	162-0017-30	2.4 mm / 96 mm / 30° Optic
■	162-1124-30	2.4 mm / 110 mm / 30° Optic
★	162-0013-30	2.7 mm / 110 mm / 30° Optic
✕	162-0018-30	2.7 mm / 187.5 mm / 30° Optic

**Shaft**



	Product Code	Description
●	162-0021-20	2.0 mm / 110 mm / 30°, stop-cock
▲	162-0031-65	2.4 mm / 96 mm / 30°, stop-cock
■	162-1131-65	2.4 mm / 110 mm / 30°, stop-cock
★	162-0021-30	2.7 mm / 110 mm / 30°, stop-cock
✕	162-0021-45	2.7 mm / 187.5 mm / 30°, stop-cock

**Trokar**



	Product Code	Description
●	162-0035-03	2.0 mm / 110 mm, sharp
▲	162-0035-22	2.4 mm / 96 mm, sharp
■	162-1135-22	2.4 mm / 110 mm, sharp
★	162-0035-14	2.7 mm / 110 mm, sharp
✕	162-0035-18	2.7 mm / 187.5 mm, sharp

**Obturator**



	Product Code	Description
●	162-0036-03	OD 2.0 mm / 110 mm, blunt
▲	162-0036-22	OD 2.4 mm / 96 mm, blunt
■	162-1136-22	OD 2.4 mm / 110 mm, blunt
★	162-0036-14	OD 2.7 mm / 110 mm, blunt
✕	162-0036-18	OD 2.7 mm / 187.5 mm, blunt

**Arthroscopy Trocar Set**

4 Sheaths, 2 Trocar pyramid tip, 2 Obturators

165-0100-00



**Rinse Cannula Set**

Complete with Trocar/Obturator and Stopcock  
3.2 mm

**165-0150-32**



**Marking Rods**

Product Code	Description
<b>165-0100-21</b>	2.1 mm
<b>165-0100-27</b>	2.7 mm
<b>165-0100-34</b>	3.4 mm



**Mini Lambotte Osteotome**

12.5 m

Product Code	Description
<b>23-3805-12</b>	3.0 mm
<b>23-3806-12</b>	4.0 mm
<b>23-3807-12</b>	6.0 mm



**Sterilization Storage System**

includes

- Sterilization Basket Standard with Lid
- Sterilization Rack for Arthroscopy Ringhandle Instrument
- Sterilization Insert Rack for Arthroscopy Hand Instrument
- Sterilization Insert Rack for Arthroscopy Flush/Rinse Instrument  
(instruments not included)


**165-5003-00**



**Sterilization Container**

See Sterilization Containers for Implants and Instruments Trays on **Page 204**.



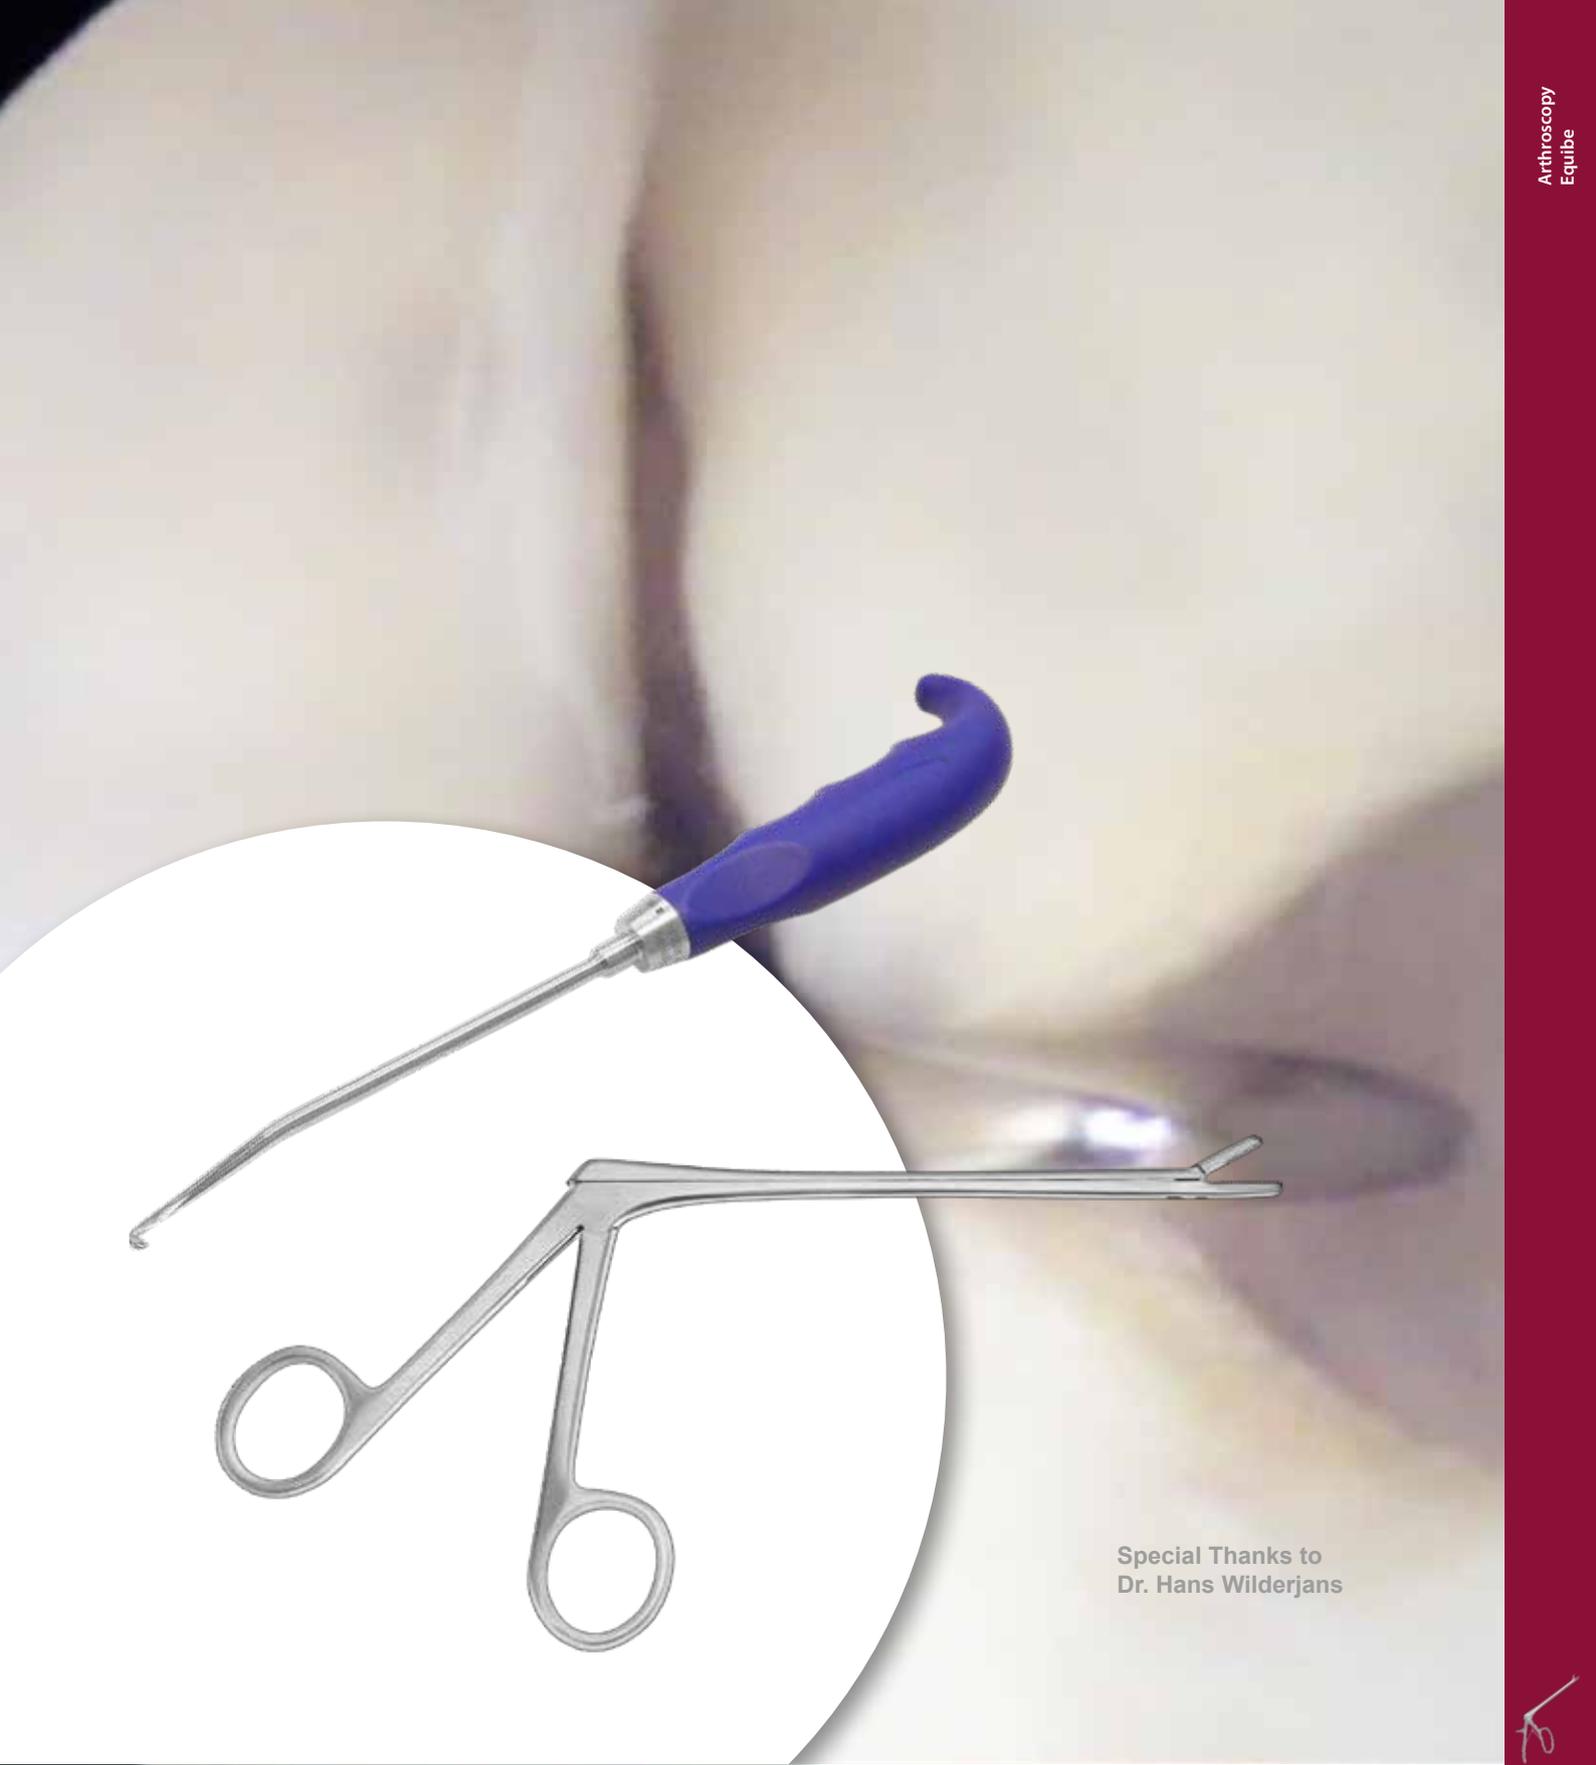

Special Thanks to  
Dr. Hans Wilderjans

# Equine **ARTHROSCOPY**

## Curved Hook Knife

### Curved Hook Knife

Design by Dr. Hans Wilderjans  
Silicone Handle

163-200-20



## Curved Hook Knife

### INDICATIONS

Chronic tenosynovitis of the digital flexor tendon sheath with thickening and constriction of the palmar annular ligament.


### GOAL

Section of a thickened and constricted annular ligament using a tenoscopic approach.

This knife is specially designed to facilitate easy cutting of the palmar annular ligament in cases of chronic tenosynovitis of the digital flexor tendon sheath in the horse.



### SPECIFICATIONS

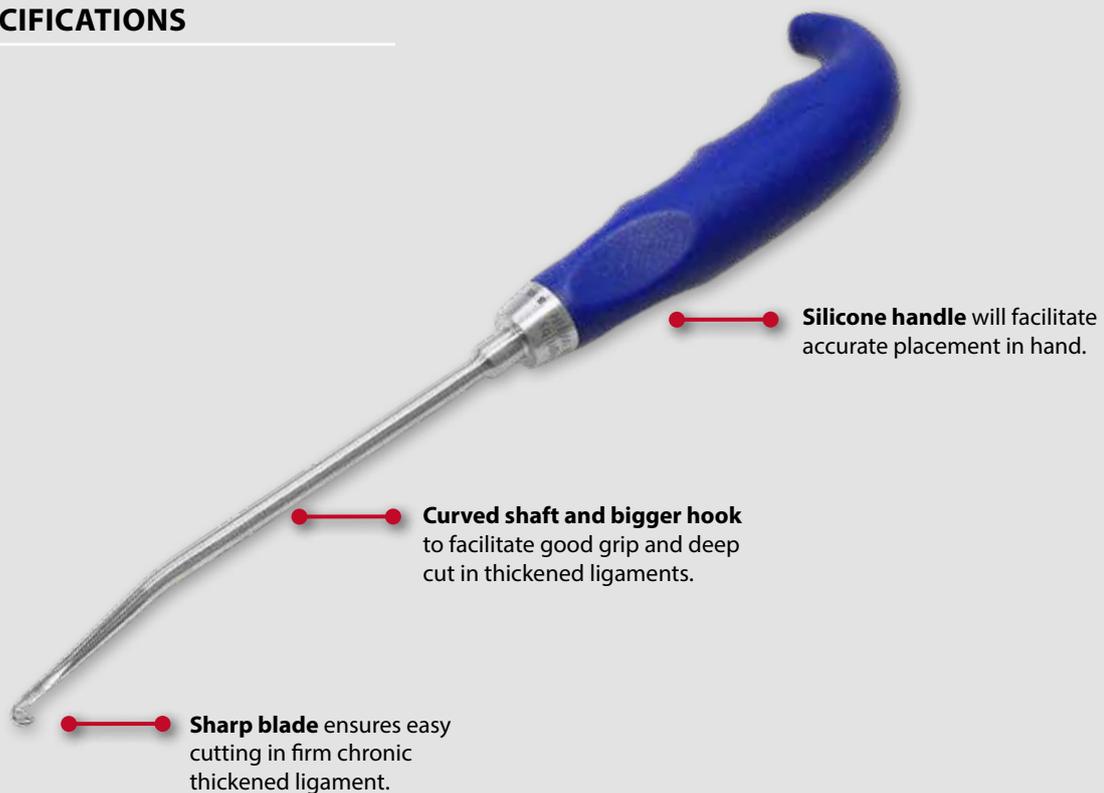

Hook Probe

Curette

Pick Probe

Banana Knife

Periosteal Elevator



**Rita Leibinger Propylux Grip**

for secure and fatigue-free working  
Sterilizable up to 134°C / 273°F

**Hook Probe**

Propylux handle blue, 225 mm, working end 110 mm, D 18

**163-600-10**



**Banana Knife**

Curved,  
Propylux handle blue, 225 mm, working end 110 mm, D 18

**163-600-11**



**Curette**

Straight  
Propylux handle blue, 225 mm, working end 110 mm, D 18

Product Code	Description
<b>163-600-12</b>	2 mm
<b>163-600-13</b>	3 mm
<b>163-600-14</b>	4 mm
<b>163-600-15</b>	5 mm



**Curette**

Curved, 45°, 5 mm  
Propylux handle blue, 225 mm, working end 110 mm, D 18

**163-600-16**



**Pick Probe**

Propylux handle blue, 225 mm, working end 110 mm, D 18

Product Code	Description
<b>163-600-17</b>	strongly curved
<b>163-600-18</b>	slightly curved



**Elevator**

Small  
Propylux handle blue, 225 mm, D 18

Product Code	Description
<b>163-600-19</b>	110 mm working end
<b>163-600-22</b>	65 mm working end



**Elevator**

Large  
Propylux handle blue, 300 mm, working end 150 mm, D 18

**163-600-20**



**Periosteal Elevator**

Propylux handle blue, 225 mm, working end 110 mm, D 18

**163-600-21**



**Hook Grasping Forceps**

2x2 teeth, long


**163-500-28**



**Hook Grasping Forceps**

Suprapatellar

**163-501-28**

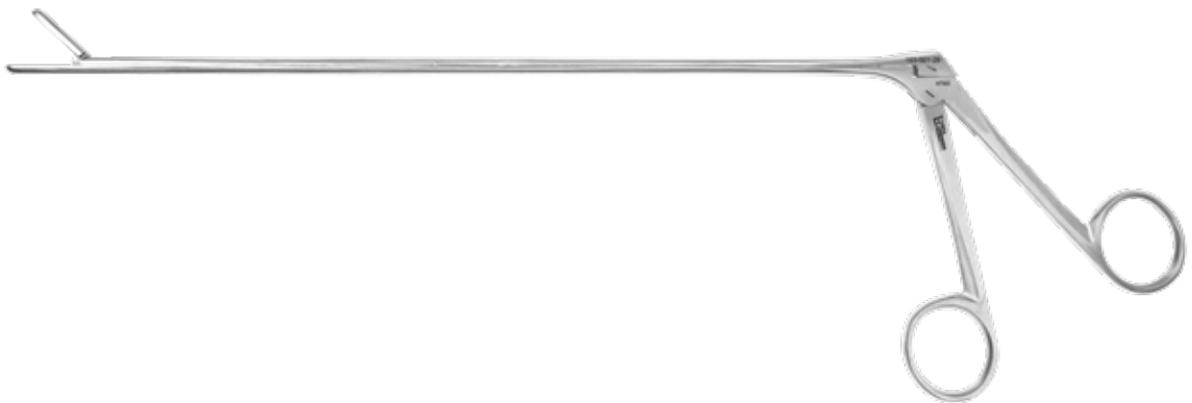

**Arthroscope**

4.0 mm, autoclave 132°/273°F,  
Stainless Steel



Product Code	Description
<b>162-0019-00</b>	0 °, 175 mm long
<b>162-0019-30</b>	30 °, 175 mm long

**Arthroscopy Shaft, OD 6.0 mm**

With 2 stop-cocks, for 4.0mm Arthroscopes 0°/30°

**162-0040-30**

**Arthroscopy Obturator**


For arthroscopy shaft 162-0040-30, blunt

**162-0040-35**




[arthroscopy.leibinger.vet](http://arthroscopy.leibinger.vet)

Arthroscopy Rongeurs

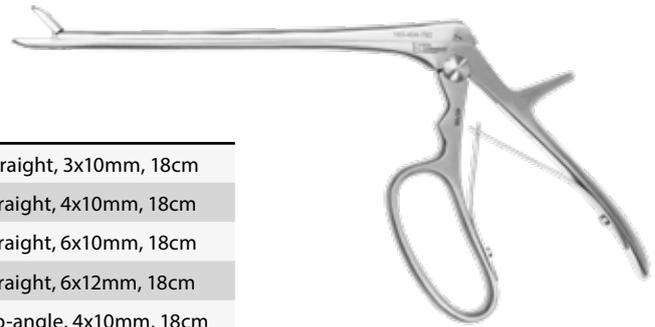


Product Code	Description
163-404-791	Ferris-Smith Arthr. Rongeur, pike shaped tip, straight, 3x10mm, 18cm
163-404-792	Ferris-Smith Arthr. Rongeur, pike shaped tip, straight, 4x10mm, 18cm
163-404-794	Ferris-Smith Arthr. Rongeur, pike shaped tip, straight, 6x10mm, 18cm
163-404-795	Ferris-Smith Arthr. Rongeur, pike shaped tip, straight, 6x12mm, 18cm
163-404-802	Ferris-Smith Arthr. Rongeur, pike shaped tip, up-angle, 4x10mm, 18cm
163-404-812	Ferris-Smi. Arthr. Rongeur, pike shaped tip, down-angle, 4x10mm, 18cm



Pike-Shaped tip

Arthroscopy Rongeurs

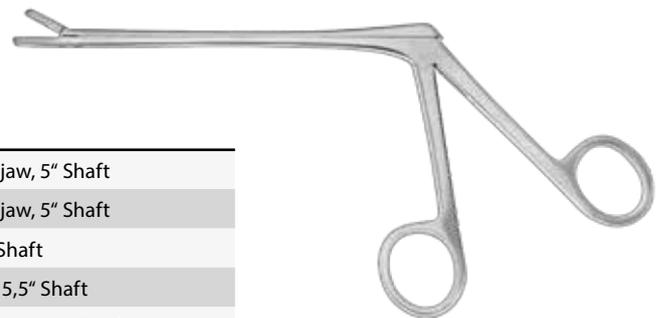

Product Code	Description
163-404-755	Schlesinger Rongeur, straight, 3x10mm serrated jaw, 5" Shaft
163-404-756	Schlesinger Rongeur, straight, 4x10mm serrated jaw, 5" Shaft
163-404-768	Wilde Ethmoid Rongeur, straight, 4mm jaw, 5,5" Shaft
163-404-782	Mcllwraith Peapod Rongeur, straight, 2.5x6mm, 5,5" Shaft
163-404-784	Mcllwraith Peapod Rongeur, up-angle, medium jaw, 5,5" Shaft




## Equine Arthroscopy Set

Set contains:

- Hook Probe
- Banana Knife
- Curettes 2,3,4 & 5 mm
- Curette curved, 5mm
- 2 pick probes, strongly and slightly curved
- 2 elevators, standard 110mm, large 150mm, short 65mm
- Dissector Periosteal Elevator
- 6 Ferris Smith Arthroscopic Rongeurs,  
(3x10, 4x10, 6x10, 6x12, 4x10 up- & 4x10 down angle)
- 5 Arthroscopic Rongeurs,  
(Schlesinger, Wilde Ethmoid, Mcllwraith Peapod)
- Hook Grasping Forceps 2x2 teeth
- Hook Grasping Forceps Suprapatellar



**163-1000-00**

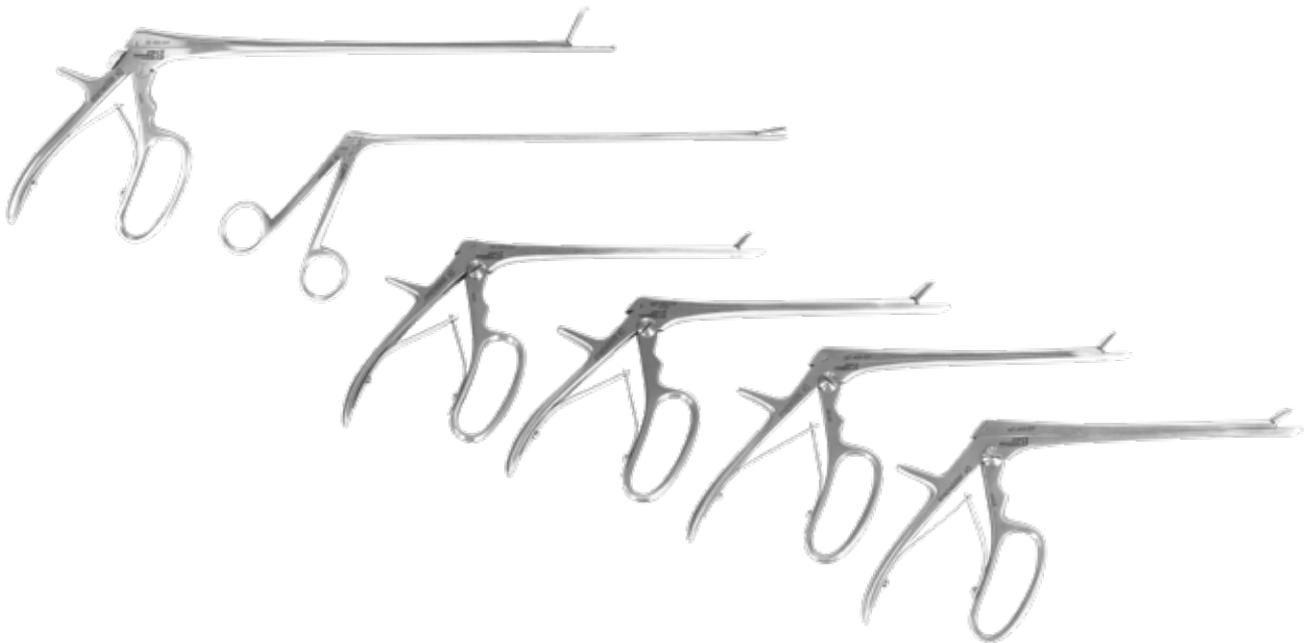



# EQUINE DENTAL

**R** RITA  
LEIBINGER  
MEDICAL

## Equine Dental Plug Set

NEW

### Titanium Equine Dental Plugs

Expertly designed to close non-healing oro-nasal and oro-sinusal fistulae in horses, these plugs provide convenient insertion through a straightforward transbuccal approach using a screwdriver. Their threaded design ensures secure and stable placement. Crafted from high-quality titanium, the RITA LEIBINGER Dental Plugs are highly biocompatible and durable.



### Equine Dental Plug Set

Set contains:

Product Code	Description	Qty
888-9500-10	Tray with Lid	1
123-3019-00	Screwdriver Shaft T30	1
123-1019-00	Screwdriver Shaft T10	1
247-0101-00	Silicone T-Handle, AO	1
247-0102-00	Screwdriver Handle, AO	1
888-9501-00	Screws for Dental Plugs, Titanium	10
888-9507-20	Equine Dental Plug, Ø7 x 20mm	2
888-9510-20	Equine Dental Plug, Ø10 x 20mm	2
888-9513-20	Equine Dental Plug, Ø13 x 20mm	2
888-9516-20	Equine Dental Plug, Ø16 x 20mm	2
888-9519-20	Equine Dental Plug, Ø19 x 20mm	2

888-9500-00

Tray without contents

888-9500-10



### Sterilization Container


See Sterilization Containers for Implants and Instruments Trays on **Page 204**.

## Equine Dental Plugs

## Screwdriver Shafts for Dental Plugs

### Equine Dental Plugs

Titanium, LeiStar, including screws

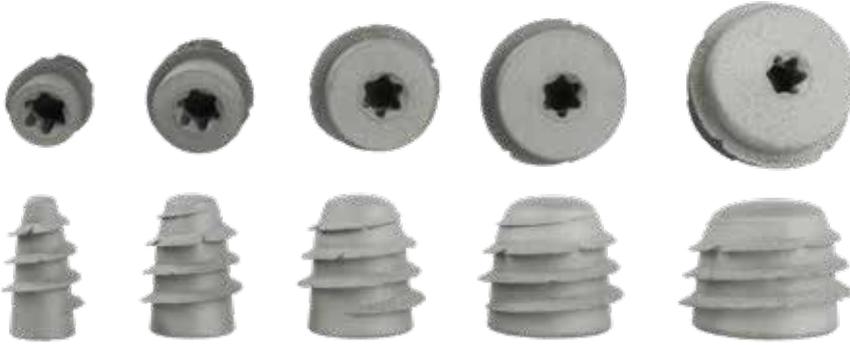

Product Code	Ø	Length
888-9507-20	7 mm	20 mm
888-9510-20	10 mm	20 mm
888-9513-20	13 mm	20 mm
888-9516-20	16 mm	20 mm
888-9519-20	19 mm	20 mm



### Screw for Dental Plugs

Titanium, LeiStar, T10, 3mm length

**888-9501-00**

### Screwdriver Shaft for Dental Plugs

T30, AO Connection, Stainless Steel, 190mm in length


**128-3019-00**



### Screwdriver Shaft for Dental Plug Screws

T10, AO Connection, Stainless Steel, 190mm in length

**128-1019-00**

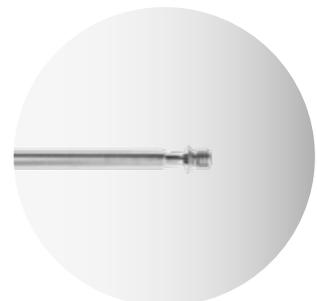

## Screwdriver T-Handle

### Screwdriver Handle

Silicone, AO-Connection  
sterilizable up to 134°C / 273°F




Product Code	Description
247-0102-00	standard, compatible with 2.7/3.5

### Screwdriver T-Handle

Silicone, AO, not cannulated  
sterilizable up to 134°C / 273°F



**247-0101-00**

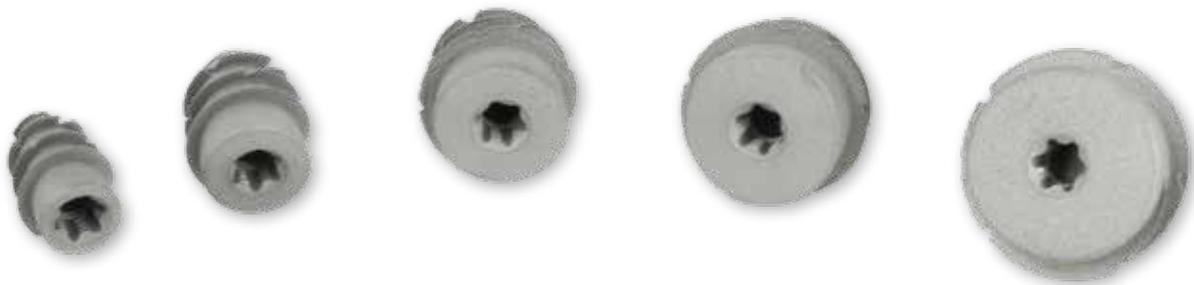



# POWER TOOLS



**Advanced function controls**

- High speed and oscillating drilling
- Low speed drilling, screw driving and tapping
- Torque limiting for screw driving
- Forward and reverse triggers
- Mode selector button with mechanical safety lock



**Handpiece**


DE SOUTTER V-MBQ-708  
0-1350 rpm  
Twin Trigger

**125-5000-00**

Compatible Batteries	Battery Housing	Battery Shield	Battery Charger
<b>125-5006-00</b> DE SOUTTER AB-703 Large Battery	125-5007-00 DE SOUTTER V-AH-703	125-5008-00 DE SOUTTER AS-703	125-5060-00 DE SOUTTER BC-708
<b>125-5055-00</b> DE SOUTTER AB-703 Small Battery	125-5056-00 DE SOUTTER V-AH-703	125-5057-00 DE SOUTTER AS-703	125-5059-00 DE SOUTTER BC-707

**Straight Case Features**

- Uses the same motor as V-MBQ-708
- Compatible with all V-MBQ-708 attachments (chucks, adapters, drivers)

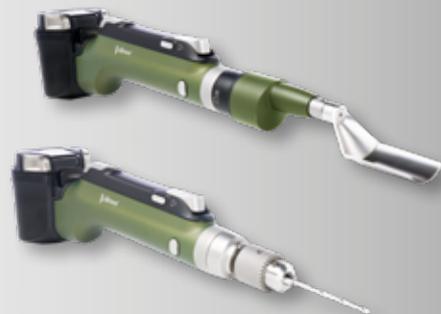

**Straight Case Modular Handpiece**

DE SOUTTER V-MBQ-807  
0-1350 rpm  
Twin Trigger

**125-5020-00**



Compatible Batteries	Battery Housing	Battery Shield	Battery Charger
<b>125-5006-00</b> DE SOUTTER AB-703 Large Battery	125-5007-00 DE SOUTTER V-AH-703	125-5008-00 DE SOUTTER AS-703	125-5060-00 DE SOUTTER BC-708
<b>125-5055-00</b> DE SOUTTER AB-703 Small Battery	125-5056-00 DE SOUTTER V-AH-703	125-5057-00 DE SOUTTER AS-703	125-5059-00 DE SOUTTER BC-707

Jacobs Chuck

Sagittal Saw Adapter

TPLO Saw Adapter

Pin Driver

**Jacobs Chuck**

DE SOUTTER V-DQ-708  
0.5 - 6.4 mm (1/4") keyed  
speed (rpm) 0 - 1350  
cannulation Ø mm 4.4

**125-5001-00**



**AO Quick-Connection Chuck**

DE SOUTTER V-DQ-708  
small A.O Synthes/ASIF  
speed (rpm) 0 - 1350  
cannulation Ø mm 2.1

**125-5002-00**



**Sagittal Saw Adapter**

DE SOUTTER V-NQ-707  
speed (cpm) 0 - 20000

**125-5003-00**



**TPLO Saw Adapter**

DE SOUTTER V-OQ-708  
oscillating saw Uses Slocum blades  
speed (cpm) 0 - 13500

**125-5004-00**

\* Saw Blade not included

**Pin Driver**


DE SOUTTER V-WQ-707  
0.7 - 4.0 mm wire capacity  
speed (rpm) 0 - 1350

**125-5005-00**



**Saw Blades**

See saw blades  
on **Page 191**.



**Twist Drill**

See Drill Bits  
on **Page 199**.



**Power Tools Tray**

See sterilizable Trays for Power  
Tools on **Page 191**.



**Advanced function controls**

- High speed and oscillating drilling
- Low speed drilling, screw driving and tapping
- Torque limiting for screw driving
- Forward and reverse triggers
- Mode selector button with mechanical safety lock



**Handpiece**

DE SOUTTER V-MBU-470  
0-1350 rpm  
Twin Trigger

**125-5050-00**

Compatible Batteries	Battery Housing	Battery Shield	Battery Charger
<b>125-5006-00</b> DE SOUTTER AB-703 Large Battery	125-5007-00 DE SOUTTER V-AH-703	125-5008-00 DE SOUTTER AS-703	125-5060-00 DE SOUTTER BC-708
<b>125-5055-00</b> DE SOUTTER AB-703 Small Battery	125-5056-00 DE SOUTTER V-AH-703	125-5057-00 DE SOUTTER AS-703	125-5059-00 DE SOUTTER BC-707

**Jacobs Chuck**

DE SOUTTER V-DU-470  
0.5 - 4.0 mm (5/32") Keyed  
speed (rpm) 0 - 1350  
cannulation Ø mm 4.1



**125-5051-00**

**AO Quick-Connection Chuck**

DE SOUTTER V-DU-470  
small A.O Synthes/ASIF  
speed (rpm) 0 - 1350  
cannulation Ø mm 2.1



**125-5052-00**

**Sagittal Saw Adapter**

DE SOUTTER V-NU-470  
speed (cpm) 0 - 20500 cpm



**125-5053-00**

**Pin Driver**

DE SOUTTER V-WU-471  
0.7 - 4.0 mm capacity  
speed (rpm) 0 - 1350

**125-5054-00**

Rechargeable Batteries

Battery Charger

ASEPTIC BATTERIES



**Large battery**

DE SOUTTER AB-703  
Battery pack 14,6 V, Capacity (mAh) 2000  
for charger 125-5060-00

**125-5006-00**



**Battery housing**

DE SOUTTER V-AH-703  
for Battery 125-5006-00  
for charger 125-5060-00

**125-5007-00**



**Sterile Funnel**

DE SOUTTER AS-703  
for Battery 125-5006-00  
for charger 125-5060-00

**125-5008-00**



**Small battery**

DE SOUTTER AB-703  
Battery pack 10,95 V, Capacity (mAh) 2000  
for charger 125-5059-00

**125-5055-00**



**Battery housing**

DE SOUTTER V-AH-703  
for Battery 125-5055-00  
for charger 125-5059-00

**125-5056-00**



**Sterile Funnel**

DE SOUTTER AS-703  
for Battery 125-5055-00  
for charger 125-5059-00

**125-5057-00**

**DE SOUTTER BC-707 SINGLE BAY CHARGER**

with 1 slot  
for Battery Type AB-703 (Product Code 125-5055-00)

**125-5059-00**

**DE SOUTTER BC-708 SINGLE BAY CHARGER**

with 1 slot  
for Battery Type AB-704 (Product Code 125-5006-00)

**125-5060-00**



\*Battery not included

**Why choose Lithium Ion battery technology?**

De Soutter Medical Lithium Ion batteries offer the surgical team and sterile services a number of tangible benefits over conventional battery technology, including:

- Li-Ion technology improves battery "capacity to weight" ratio by around 100% when compared to NiMH or NiCad chemistries
- Significantly extends the usable run time of the power tool
- Eliminates 'memory effect' normally associated with other battery types
- Unique fuel gauge incorporated within De Soutter Medical Li-Ion batteries allows the surgical team to instantly assess the battery capacity both before and during use




Saw Blades (all)

**Sawblades - „Samoy Rapid-Cut“**

extreme cutting precision optimum performance protection against wear and tear titanium nitride\*




Colibri




Aesculap



Linvatec-Hall



AO/Synthes





DeSoutter



TERRIER



HORNET

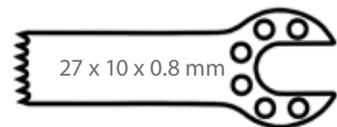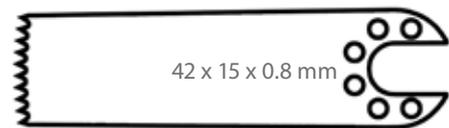

Standard	Length x Width x Cutting Thickness			
for Connection	50 x 20 x 0.8 mm	42 x 15 x 0.8 mm	35 x 12 x 0.8 mm	27 x 10 x 0.8 mm
Colibri	102-1420-50	102-1414-42	102-1411-35	102-1411-27
Aesculap		102-1714-42	102-1711-35	102-1711-27
Linvatec-Hall	102-1520-50	102-1514-42	102-1511-35	102-1511-27
AO/Synthes	102-1620-50	102-1614-42	102-1611-35	102-1611-27
	50 x 19.8 x 0.6 mm	46 x 15 x 0.6 mm	25 x 10 x 0.6 mm	27 x 6.4 x 0.6 mm
DeSoutter	102-16520-50	102-16515-46	102-16510-25	102-16506-27
		40 x 16 x 0.7 mm	40 x 12 x 0.7 mm	
TERRIER		102-1916-40	102-1912-40	
		18 x 6 x 0.3 mm	24 x 9 x 0.3mm	
HORNET		102-2026-18	102-2026-24	

„Petite“	Product Code	Length x Width x Cutting Thickness
Colibri	102-1211-30	30x11x0.6mm
Aesculap	102-1212-25	25x10x0.7mm
Linvatec-Hall	102-1213-25	25.5x9.4x0.65mm
AO/Synthes	102-1210-25	25x10x0.6mm

\*Titanium Nitride (TiN) is one of the hardest and toughest materials in the medical field. TiN coated Saw-Blades lasts up to 5 times longer.

TPLO Saw Blades

Sterilization Tray for Power Tools

TPLO Saw Blades

with triangle connection

Leibinger TPLO Sawblades are coated with Titanium Nitride (TiN). Titanium Nitride (TiN) is one of the hardest and toughest materials in the medical field.

Product Code	Width
102-2100-09	09 mm
102-2100-12	12 mm
102-2100-15	15 mm
102-2100-18	18 mm
102-2100-21	21 mm
102-2100-24	24 mm
102-2100-27	27 mm
102-2100-30	30 mm
102-2100-33	33 mm



Sterilization Tray for Power Tools

For storage and sterilization of Power Tools  
Tray with lid, without contents

Compatible with DeSoutter V-MBQ-708 and V-MBQ-807 (Product Code: 125-5000-00 and 125-5020-00) and attachments

**125-5000-10**

Compatible with DeSoutter V-MBU-470 (Product Code 125-5050-00) and attachments

**125-5050-10**



*\*Tray with lid and silicone holders only.  
Power Tools and other contents not included.*



**NEW**

**HEKADRILL**  
**Ultimate Precision**

Developed with innovation and precision in mind

- High speed motor up to 85,000 rpm
- Allows high torque/low speed control (min. 200 rpm)
- Advanced motor control for comfort during extended use, and with minimal heat gain
- Adjustable bur exposure lengths
- Adjustable acceleration and braking functionality



**hekaDrill Handpiece**

DE SOUTTER HDS-121 (103347)  
200-85,000 rpm  
Cable length 4m

**125-6050-00**



**hekaDrill Attachment, Straight**

DE SOUTTER S-C07 (103360)  
Length 70mm, Bur Size 2.38 mm

**125-6051-00**



**hekaDrill Power Console**

DE SOUTTER PC-121 (103318)  
with irrigation

**125-6052-00**

**Mains Power Cable**

DE SOUTTER 8300  
3m long, wit Euro plug

**125-6052-01**



**Power Console with Irrigation**

- Simultaneous dual handpiece operation
- Adjustable acceleration and braking functionality
- Integrated and customisable irrigation control with anti-drip mode
- 200+ user profiles can be stored and easily accessed
- Rings illuminate to indicate port status for ease of use

hekaDrill Foot Pedal

hekaDrill Irrigation Kit

hekaDrill Burs

**Foot Pedal, wired**

DE SOUTTER MFP-120 (103556)  
with A or B tool selection and foot pedal underlighting

**125-6053-00**



**Connecting and Charging Cable**

DE SOUTTER 103597  
4m long, connects and charges the foot pedals via power console

**125-6053-01**



**hekaDrill Sterile Irrigation Kit**

DE SOUTTER S101461  
Box of 5

**125-6054-00**




**Fluted Bur, Ball**

High Speed Bur, Fluted Ball Gold

Product Code	DE SOUTTER Product Code	Size (mm)	Shaft Ø (mm)	Length (mm)
<b>148-0650-20</b>	C07-02031	<b>2.0</b>	2.38	70
<b>148-0650-30</b>	C07-03031	<b>3.0</b>	2.38	120
<b>148-0650-50</b>	C07-05031	<b>5.0</b>	2.38	120

\* More sizes available on request

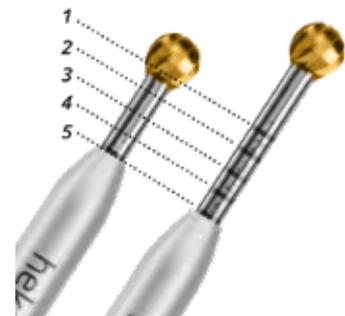

**Fluted Bur, Match**

High Speed Bur, Fluted Match Gold

Product Code	DE SOUTTER Product Code	Size (mm)	Shaft Ø (mm)	Length (mm)
<b>148-0651-17</b>	C07-01734	<b>1.7</b>	2.38	70
<b>148-0651-30</b>	C07-03034	<b>3.0</b>	2.38	70

\* More sizes available on request



\* All Burs allow for 5 possible exposure positions offering total flexibility and reduced inventory costs



# S.O.S. Screw Extraction



**CASE 1**

## Stripped screw head

If the screw head is stripped and the screwdriver is not engaging into the head of the screw

- 1 Choose a conical extractor that corresponds to the diameter of the screw. Choose one size larger when the screw drive is severely damaged.
- 2 Attach the conical extractor to the AO handle and insert it into the screw head recess. Applying slight pressure, turn the device counterclockwise.
- 3 As soon as the extractor fully engages, the screw will start to move. Continue turning until screw is completely removed.



**CASE 2**

## Screw Head broke off

Screw head broke off and the screw shaft protrudes from the bone

- 1 Attach the extraction bolt to the AO Handle and place it on top of the protruding screw shaft.
- 2 Applying slight pressure, turn the device counterclockwise.
- 3 As soon as the extraction bolt engages and sufficient grip is achieved, the screw will start to move. Continue turning until the screw shaft is completely removed.




**CASE 3**

## Broken screw shaft is below cortical surface of the bone

- 1 Either use a gouge chisel or a hollow reamer. Choose the correct diameter that corresponds to the screw size. Remove surrounding bone to expose enough of the screw shaft. A few initial threads is often sufficient.
- 2 Attach the corresponding extraction bolt to the AO Handle and place on top of the exposed screw shaft.
- 3 Applying slight pressure, turn the device counterclockwise.
- 4 As soon as the extraction bolt engages and sufficient grip is achieved, the screw will start to move. Continue turning until the screw shaft is completely removed.

# Instruments

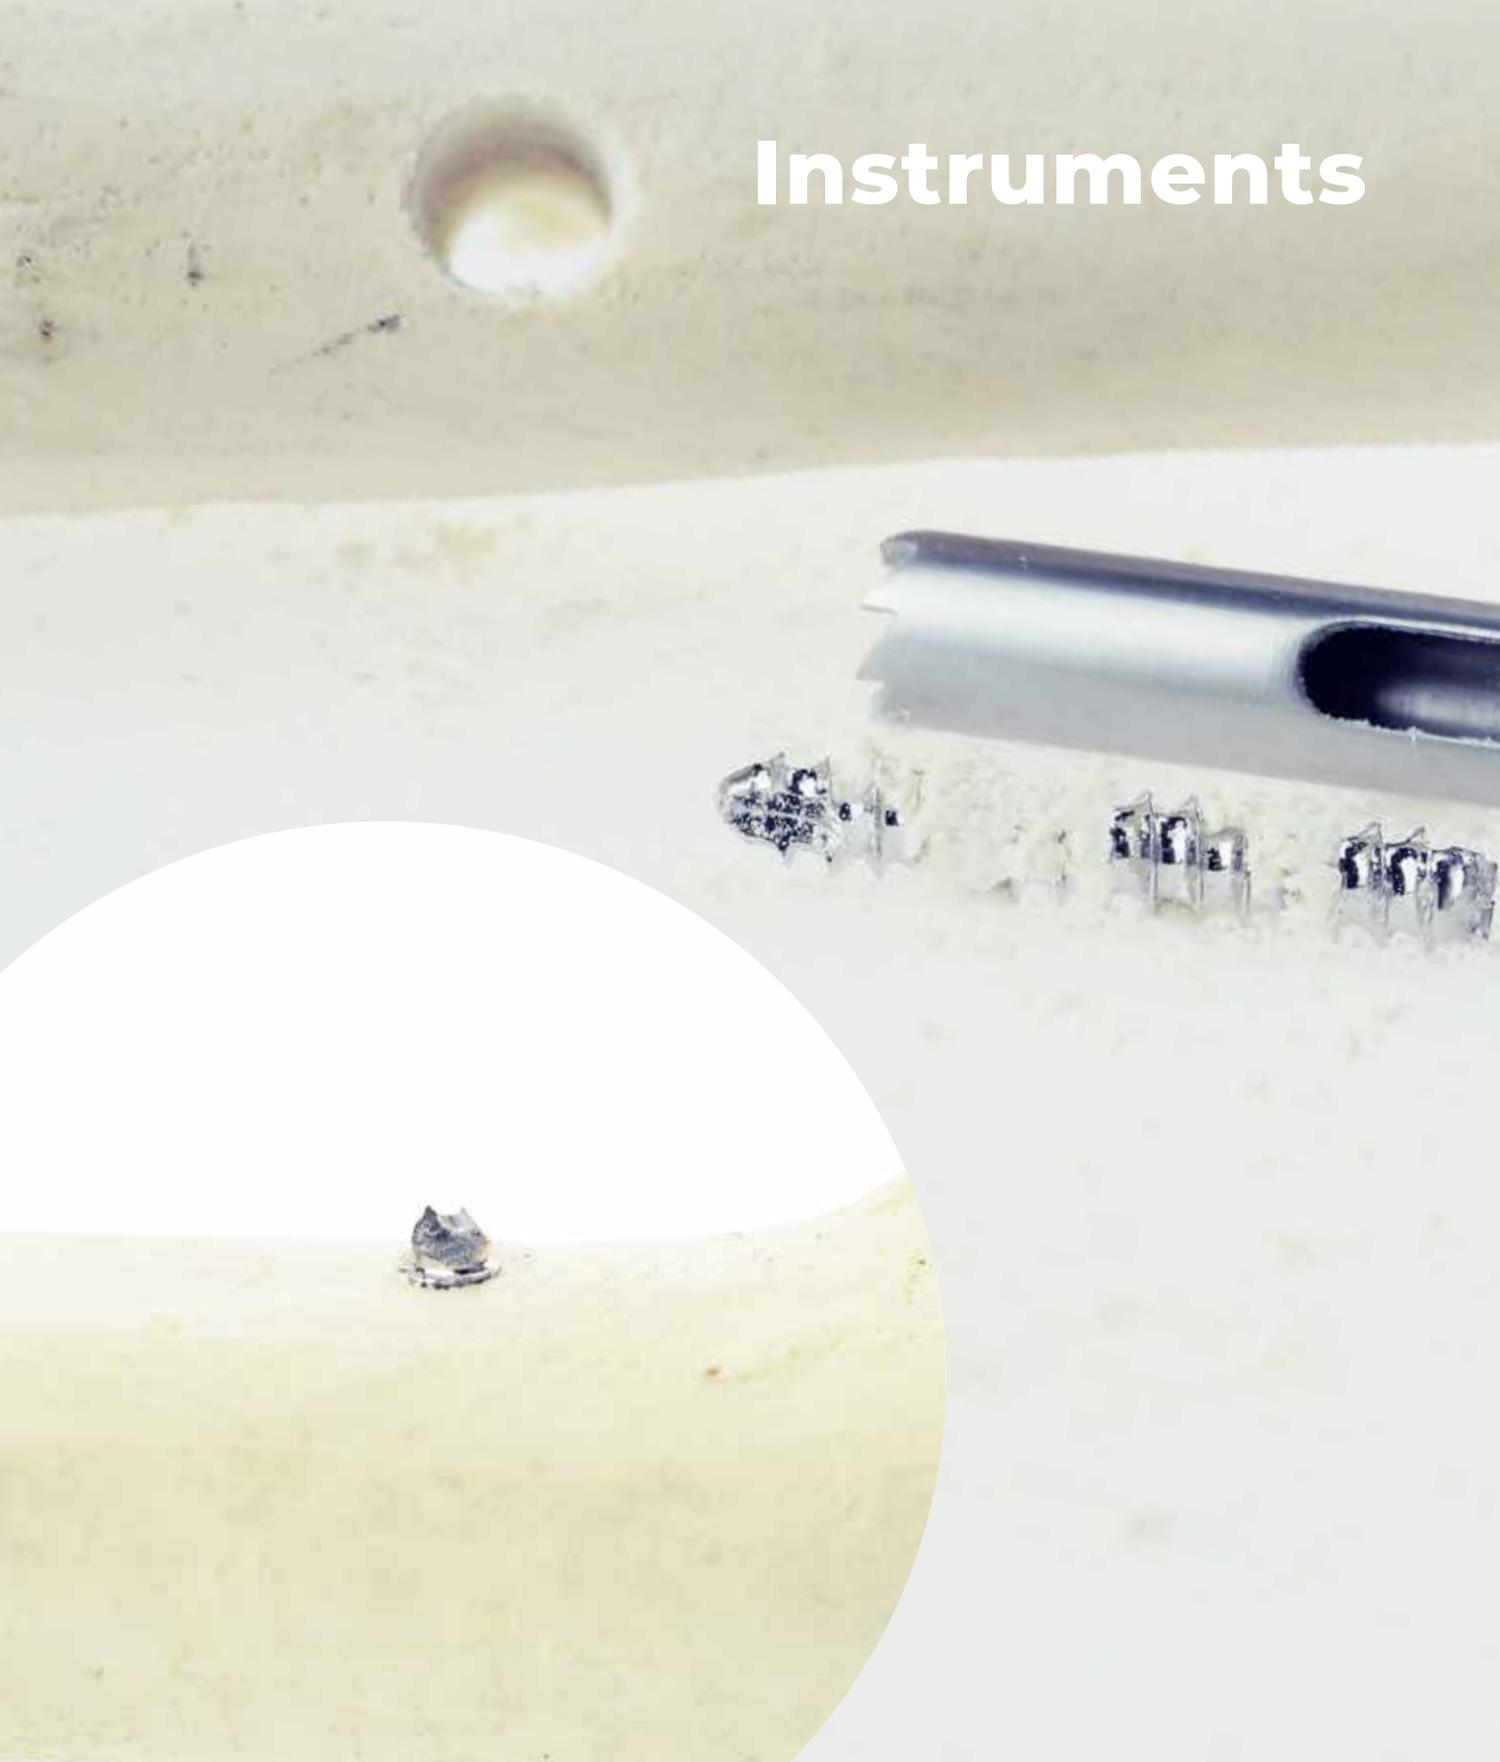

## SCREW REMOVAL



S.O.S. - Screw Removal Set

247-0000-00

Product Code	Description
150-0863-00	Wire Box for 24 Inserts, with Lid
150-0864-00	Wire Box for handles
247-0101-00	Silicone T-Handle, AO
247-0102-00	Screwdriver Handle Silicone, straight, AO
128-0300-15	Bone Pick, 15 cm
247-0110-00	Screwdriver Shaft LeiStar AO, T4, 1,28
128-1520-15	Screwdriver Shaft LeiStar AO, T6, 1,6 mm
247-0112-00	Screwdriver Shaft LeiStar AO, T7, 1,99 mm
247-0113-00	Screwdriver Shaft LeiStar AO, T8, 2,31 mm
247-0114-00	Screwdriver Shaft LeiStar AO, T9, 2,5 mm
247-0115-00	Screwdriver Shaft LeiStar AO, T10, 2,74 mm
247-0116-00	Screwdriver Shaft LeiStar AO, T15, 3,27 mm
247-0117-00	Screwdriver Shaft LeiStar AO, T25, 4,43 mm
247-0120-00	Screwdriver Shaft Cross Drive AO, CD1.0/1.2
247-0121-00	Screwdriver Shaft Cross Drive AO, CD 1.5/1.7
247-0122-00	Screwdriver Shaft Cross Drive AO, CD 2.0/2.3
247-0130-00	Screwdriver Shaft Hexagonal AO, 1.5mm
247-0131-00	Screwdriver Shaft Hexagonal AO, 2.5mm
247-0132-00	Screwdriver Shaft Hexagonal AO, 3.5mm
247-0133-00	Screwdriver Shaft Hexagonal AO, 2.0mm
247-0140-00	Extraction Bolt, AO for Screws 1.5 mm
247-0141-00	Extraction Bolt, AO for Screws 2.0 mm
247-0142-00	Extraction Bolt, AO for Screws 2.7 mm
247-0143-00	Extraction Bolt, AO for Screws 3.5/4.0 mm
247-0150-00	Conical Extractor, AO 1.5 / 2.0 mm
247-0151-00	Conical Extractor, AO 2.7 / 3.5 / 4.0 mm
247-0152-00	Conical Extractor, AO 4.5 / 5.0 / 6.5 / 7.0mm
247-0160-00	Hollow Reamer 1.5 / 2.0 mm
247-0161-00	Hollow Reamer 2.7 / 3.5 / 4.0 mm



**Sterilization Container**

See Sterilization Containers for Implants and Instruments Trays on **Page 204**.

# Instruments

Miscellaneous

Instruments



## GENERAL INSTRUMENTS



**Screw Racks**  
(without screws)

Product Code	Description
150-0515-00	for 1.5 mm screws
150-0520-00	for 2.0 mm screws
150-0524-00	for 2.4 mm screws
150-0527-00	for 2.7 mm screws
150-0535-00	for 3.5 mm screws
150-4027-00	for 2.7mm screws (extended: 6-52mm)
150-4035-00	for 3.5 mm screws (extended: 6-70mm)



**Mini-AO QC Screwdriver 1.5/2.0**

Handle

**128-0807-00**

Shaft

**128-0905-15**

Holding Sleeve

**128-0905-17**



**Screwdriver 2.4 Propylux Hex**

Without Holding Sleeve, Propylux handle

**128-0911-25**



**Screwdriver Handle**

Silicone, AO-Connection  
sterilizable up to 134°C / 273°F

Product Code	Description
247-0103-00	compact, compatible with 2.0/2.4
247-0102-00	standard, compatible with 2.7/3.5



**Torque Limiting Screwdriver Handle**

Torque 3 Nm  
Silicone, AO, sterilizable up to 134°C / 273°F

**247-0104-00**



## Drill Bits (all)

## Drill Guides (all)

## Drills with Round Shaft

Product Code	Ø (mm)	Length (mm)
148-0080-07	0.7	45
148-0080-10	1.0	45
148-0080-11	1.1	45
148-0180-11	1.1	85
148-0080-15	1.5	70
148-0180-15	1.5	130
148-0080-18	1.8	125

## Drills with AO Shaft

Product Code	Ø (mm)	Length (mm)
148-0081-07	0.7	72 / 47
148-0081-10	1.0	72 / 47
148-0081-11	1.1	60 / 35
148-0181-11	1.1	85 / 60
148-0081-15	1.5	85 / 60
148-0181-15	1.5	110 / 85
148-0081-18	1.8	125 / 25

## Drills with AO Shaft, cannulated

Product Code	Ø (mm)	Length (mm)	Cannulation Ø (mm)
148-0084-18	1.8	95	1.1
148-0084-23	2.3	95	1.1
148-0084-27	2.7	125	1.6
148-0084-38	3.8	125	1.6

## Drill Guide

Standard

Product Code	Size (mm)
164-0070-20	1.1/1.5
164-0070-24	1.8/2.0
164-0070-27	2.7/2.0
164-0070-35	3.5/2.5

## Drill Guide

Neutral / load

Product Code	Description
164-0071-15	for screws Ø 2.0 mm and drill Ø 1.5 mm
128-2418-24	for screws Ø 2.4 mm and drill Ø 1.8 mm
128-2720-27	for screws Ø 2.7 mm and drill Ø 2.0 mm
128-2535-35	for screws Ø 3.5 mm and drill Ø 2,5mm



Product Code	Ø (mm)	Length (mm)	Price
148-0080-20	2.0	85	
148-0080-25	2.5	95	
148-0080-27	2.7	85	
148-0080-30	3.0	100	
148-0080-32	3.2	180	
148-0080-35	3.5	180	
148-0080-45	4.5	180	



self-centering

Product Code	Ø (mm)	Length (mm)	Price
148-0081-20	2.0	100 / 75	
148-0081-25	2.5	110 / 85	
148-0081-27	2.7	125 / 100	
148-0081-30	3.0	100 / 85	
148-0081-32	3.2	145 / 120	
148-0081-35	3.5	110 / 85	
148-0081-45	4.5	195 / 170	



Locking Drill Guide

Product Code	Description
164-0010-00	for 1.0 mm Screws, 0.7 mm Drill
164-0013-00	for 1.3 mm Screws, 1.0 mm Drill
Product Code	Description
164-0015-00	for 1.5 mm Screws, 1.1 mm Drill
164-0020-00	for 2.0 mm Screws, 1.5 mm Drill
Product Code	Description
164-2000-00	for 2.0 mm screws, 1.5 mm Drill
164-2400-00	for 2.4 mm screws, 1.8 mm Drill
164-2700-00	for 2.7 mm screws, 2.0 mm Drill
164-3500-00	for 3.5 mm screws, 2.5 mm Drill



Screwdriver Shaft Hex

AO connection, (Holding Sleeve recommended)

Product Code	Description
128-0900-15	for 1.5/2.0 mm screws, 100 mm long
128-0900-20	for 2.4 mm screws, 100 mm long
134-0900-24	for 2.4 mm screws, 130 mm long
128-0900-25	for 2.7 / 3.5 mm screws, 100 mm long



Holding Sleeve

for Hexagonal Screwdriver Shafts

Product Code	Size
128-0940-24	2.0 / 2.4 mm
128-0940-25	2.7 / 3.5 mm



Screwdriver Shaft LeiStar

AO connection, self-holding  
(no Holding Sleeve needed)

Product Code	Description
128-1013-00	T5, for 1.0 mm Screws, 60 mm in length
128-1520-15	T6, for 1.5 mm Screws, 60 mm in length
128-1520-20	T8, for 2.0 / 2.4 mm screws, 60 mm in length
128-2024-08	T8, for 2.0 / 2.4 mm screws, 100 mm in length
128-2735-10	T10, for 2.7 / 3.5 mm screws, 100 mm in length
134-0800-27	T10, for 2.7 / 3.5 mm screws, 135 mm in length



## Depth Gauge (all)

## Bending Irons AO Type (all)

### Screwdriver Shaft LeiStar, cannulated

AO connection



Product Code	Description
128-2431-06	2.4 mm, 90mm, cannulated, T6 for 2.4 / 3.1 mm screws
128-3039-08	3.0 mm, 90mm, cannulated, T8 for 3.0 / 3.9 mm screws
128-4050-10	4.0 mm, 90mm, cannulated, T10 for 4.0 / 5.0 mm screws
128-5060-15	5.0 mm, 90mm, cannulated, T15 for 5.0 / 6.0 mm screws



### Depth Gauge



Product Code	Description	Compatibility
164-1013-20	150mm in length, scale up to 20mm	for 1.0/1.3/1.5 mm screws
164-1520-20	150mm in length, scale up to 40mm	for 1.5/2.0/2.4 mm screws
164-2735-60	150mm in length, scale up to 60mm	for 2.4/2.7/3.5 mm screws

### Screw Depth Gauge, cannulated

for K-Wires up to  $\varnothing$  1.6, cannulated 150



164-1600-00



### Bending Irons AO Type 1.5/2.0

130 mm, Pair

128-0881-15



### Bending Irons AO Type 2.7/3.5/4.5

140mm, Pair

Product Code	Description
128-0880-27	right
128-0881-27	left



### Plate Holding Forceps

90 mm, curved

164-0050-09



### Plate Holding Forceps

17 cm, angulated

164-0051-17




Bone Holding Forceps

Bone Plate Holding Forceps with Drill Guide

**LEIKUTA Bone Plate Holding Forceps**

with spin lock

Product Code	Description
<b>128-0538-13</b>	135 mm, 45 mm working end, angled up
<b>128-0539-13</b>	140 mm, 45 mm working end, straight

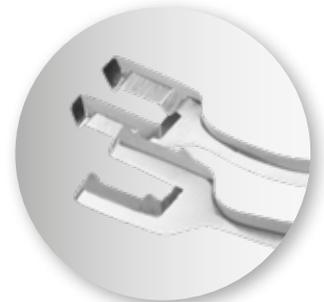

**Bone Holding Forceps**

with spin lock


Product Code	Description
<b>128-0544-03</b>	140 mm, 3 mm working end, curved
<b>128-0544-07</b>	140 mm, 7 mm working end, curved



**Bone Plate Holding Forceps with Drill Guide**

with spin lock

Product Code	Description
<b>128-0540-14</b>	140 mm, for 1.5mm drill, for 2.0mm screws
<b>128-0540-15</b>	150 mm, for 1.8/2.0mm drill, for 2.4/2.7mm screws
<b>128-0540-16</b>	155 mm, for 2.5mm drill, for 3.5mm screws

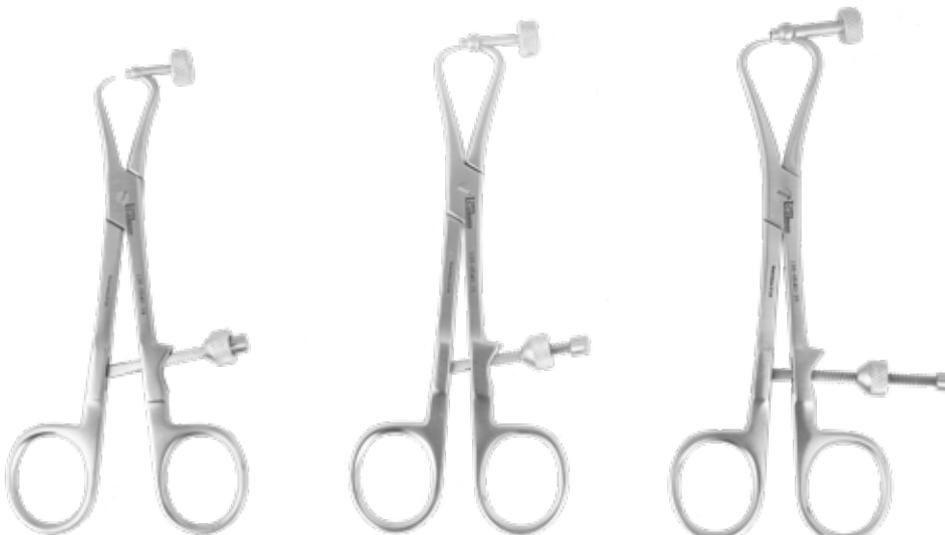

Forceps

Bone Reduction Forceps

**Bone Holding / Reduction Forceps**

Curved, with spin lock



Product Code	Description
128-0541-09	95 mm, with 2 stepped working ends
128-0541-14	135 mm, with 1 sharp and 1 stepped working end



**Bone Holding / Reduction Forceps**

135 mm, curved, with 2 sharp pointed working ends and spin lock

128-0543-13



**Bone Holding Forceps**

21.5 cm, with spin lock

128-0525-21



## Sterilization Container




### Sterilization Container

for Trays

Product Code	Description
150-5401-30	312 x 189 x 134 mm, fits 2 trays, blue lid
150-5402-30	312 x 189 x 134 m, fits 2 trays, green lid
150-5401-00	310 x 190 x 100 mm, fits 1 tray only, blue lid
150-5402-00	310 x 190 x 100 mm, fits 1 tray only, green lid

\* More sizes and colors available upon request

# Instruments

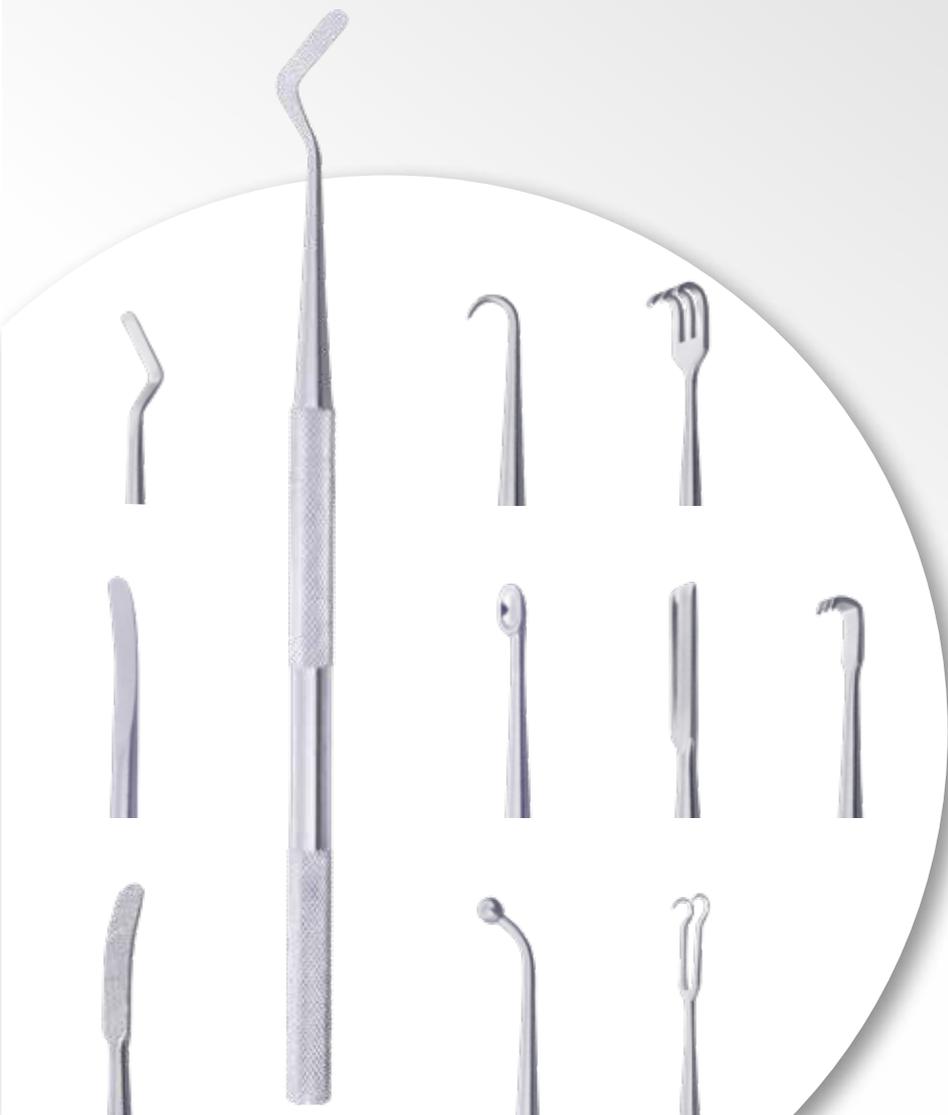

## MICRO SURGERY





**Original Size (15 cm)**

The Small Bone Orthopedic Instrument are offered in 70 various Instruments, and will offer surgeons the choice to create their own SBOI Set.

We offer the SBOI Sterilization Tray for 5 – 10 and 20 Instruments.

**Bone Lever**

Curved up, 3 mm tip



**170-1038-03**

**Bone Lever**

Curved side, 3mm tip



**170-1037-03**

**Bone Hook**

Sharp 1 prong



**170-1170-01**

**Bone Hook**

Blunt 1 prong



**170-1225-07**

**Langenbeck**

Langenbeck Retractor



Product Code	Description
<b>170-1235-06</b>	10x6 mm
<b>170-1236-04</b>	11x4 mm

**Periosteal Elevator**

Periosteal Elevator



Product Code	Description
<b>170-1025-02</b>	slight cvd. 2mm tip
<b>170-1029-06</b>	slight cvd. 6mm tip
<b>170-1030-07</b>	slight cvd. 7mm tip
<b>170-1031-08</b>	slight cvd. 8mm tip

**Bone Curette**

**Gouge**

**Bone File**

**Bone Curette**

Bone Curette

Product Code	Description
170-1040-02	2 mm
170-1045-03	3 mm



Product Code	Description
170-1050-04	4 mm
170-1055-05	5 mm



**Gouge**

Product Code	Description
170-1082-02	2 mm tip
170-1083-03	3 mm tip
170-1084-04	4 mm tip
170-1085-05	5 mm tip
170-1086-06	6 mm tip



Product Code	Description
170-1087-07	7 mm tip
170-1088-08	8 mm tip
170-1090-10	10 mm tip
170-1092-12	12 mm tip

**Bone File**

Straight, fine

Product Code	Description
170-1114-04	4 mm wide, straight, fine
170-1115-06	6 mm wide, straight, fine
170-1120-06	6 mm wide, straight, fine



**Bone File**

Curved, coarse

Product Code	Description
170-1104-04	4 mm wide, curved, coarse
170-1105-06	6 mm wide, curved, coarse



**Bone File**

Curved, fine

Product Code	Description
170-1124-04	4 mm wide, curved, fine
170-1125-06	6 mm wide, curved, fine



## Bone Awl

## Bone Packer

## Bone Tamper

## Joseph Hook

### Bone Awl

Product Code	Description
170-1135-05	5 mm tip
170-1137-25	2,5 mm tip



### Bone Packer

Ball tip

Product Code	Description
170-1155-02	2 mm ball tip
170-1156-03	3 mm ball tip
170-1157-04	4 mm ball tip
170-1158-05	5 mm ball tip



### Bone Tamper

Round Handle, 15 cm

Product Code	Description
170-1140-01	Bone Tamper, 1 mm tip
170-1142-02	Bone Tamper, 2 mm tip
170-1145-03	Bone Tamper, 3 mm tip
170-1146-04	Bone Tamper, 4 mm tip
170-1150-05	Bone Tamper, 5 mm tip



### Joseph Hook

2-prong

Product Code	Description
170-1211-02	Joseph Hook, sharp, 2-prong, 2 mm wide
170-1210-03	Joseph Hook, sharp, 2-prong, 3 mm wide
170-1216-04	Joseph Hook, blunt, 2-prong, 4 mm wide
170-1215-06	Joseph Hook, sharp, 2-prong, 4 mm wide
170-1212-07	Joseph Hook, sharp, 2-prong, 7 mm wide
170-1218-05	Joseph Hook, sharp, 2-prong, 8 mm wide



## Senn Miller Hook

## Retractor

## Scalpel Handle

## Senn Miller Hook

Product Code	Description
170-1220-08	sharp, 3-prong, 8 mm curved, 11 mm wide
170-1222-08	blunt, 3-prong, 8 mm curved, 11 mm wide
170-1223-08	sharp, 2-prong, 8 mm curved, 7 mm wide



## Meyerding Retractor

Product Code	Description
170-1232-04	6x4 mm
170-1234-04	10x4 mm
170-1233-04	6x4 mm, concave



## Cushing Retractor

No. 3, straight

Product Code	Description
170-1266-06	6 mm, rigid
170-1268-08	8 mm, rigid, concave
170-1269-08	8 mm, rigid, flat
170-1270-10	10 mm, rigid
170-1273-12	12 mm, rigid



## Hohmann Retractor

Product Code	Description
170-1005-04	4 mm tip
170-1005-06	6 mm tip
170-1010-09	9 mm tip



## Scalpel Handle

Product Code	Description
170-1305-03	No. 3, angled
170-1300-03	No. 3, straight



Osteotome



Product Code	Description
170-1062-02	2 mm tip
170-1063-03	3 mm tip
170-1065-05	5 mm tip
170-1066-06	6 mm tip

Product Code	Description
170-1067-07	7 mm tip
170-1070-10	10 mm tip
170-1072-12	12 mm tip

Instrument cases

Instrument Cassette #10

for 10 Instruments

150-0300-10





Rita Leibinger Essentials

RL X-RAY Markers "Rita Leibinger"-Design

With 2.0 cm scale, 0.5 cm steps

100-0000-02




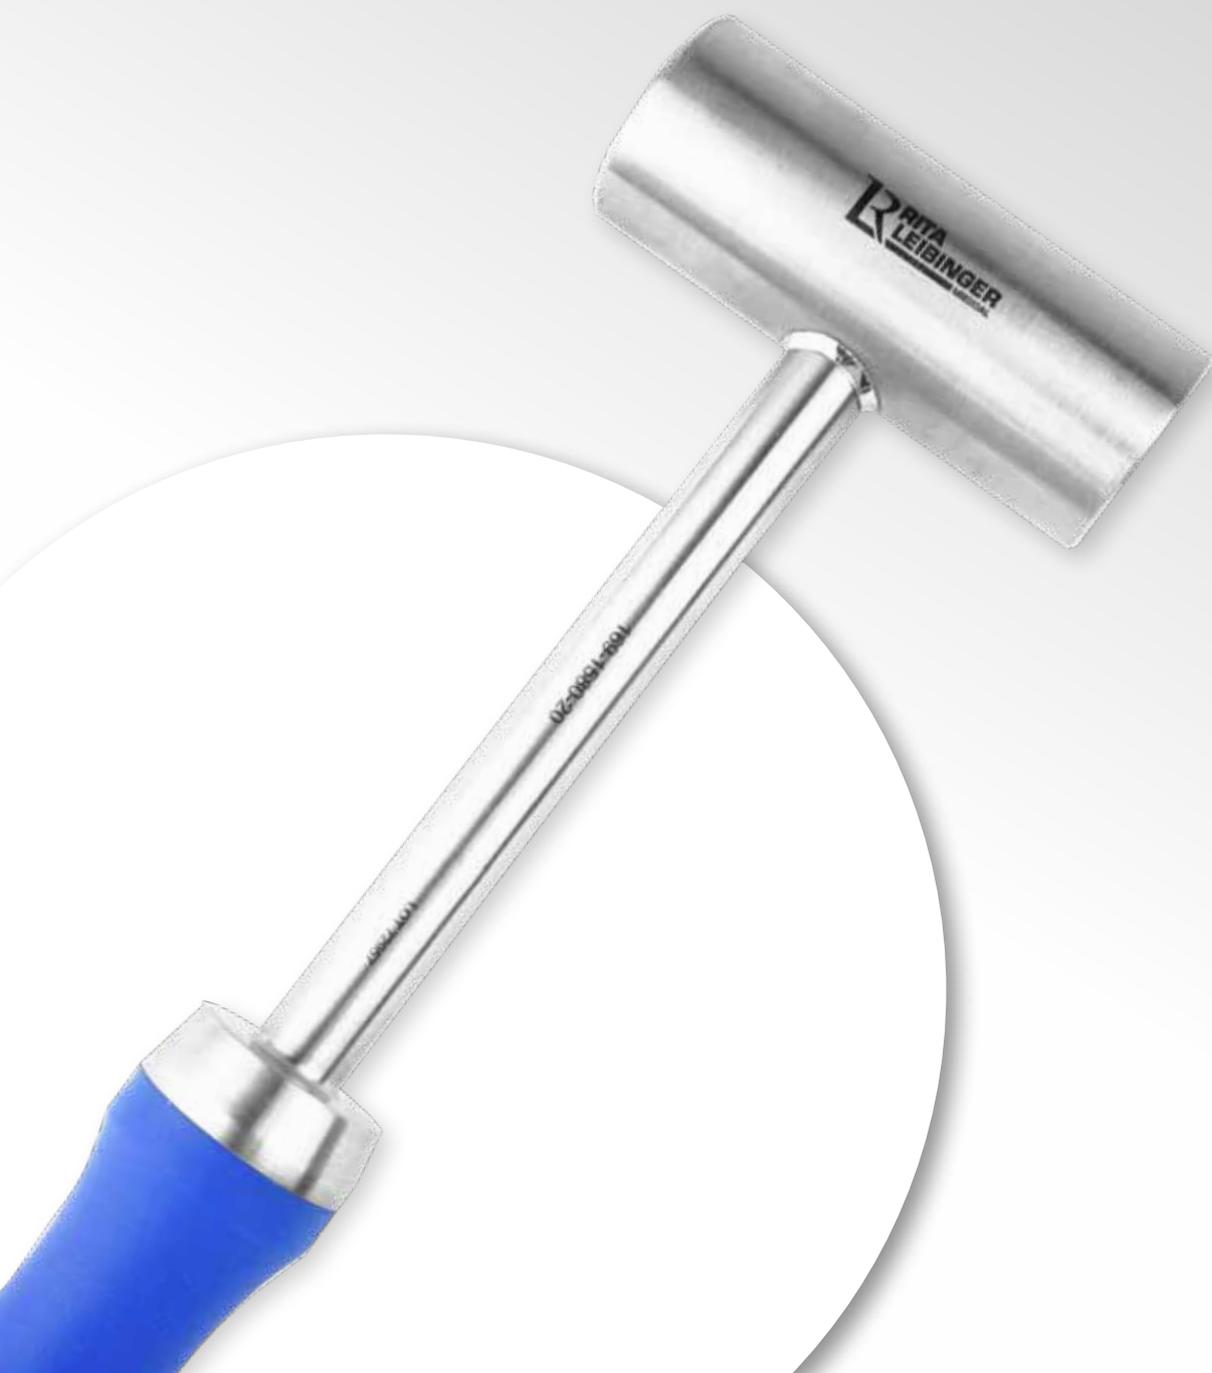

# SULCOPLASTY



## Sulcoplasty Set

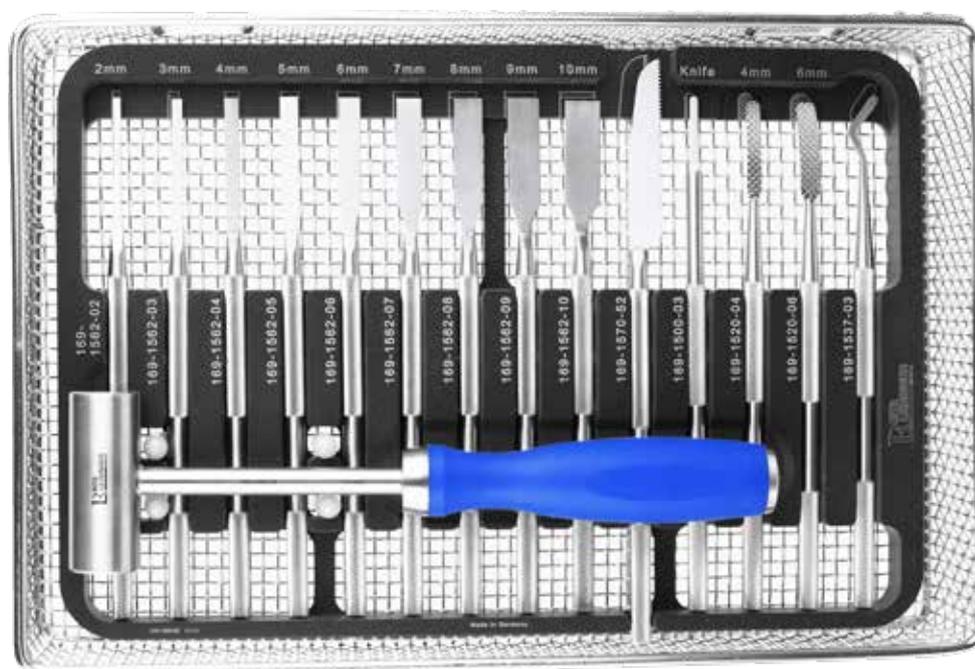

### Sulcoplasty Set

**169-1500-00**

Tray without contents

**169-1500-01**

Product Code	Description	Qty
<b>169-1500-01</b>	Sulcoplasty Instrument Tray (without contents)	1
<b>169-1500-03</b>	Sulcoplasty Scalpel Handle, No. 3, 16 cm, straight	1
<b>169-1537-03</b>	Sulcoplasty Bone Lever, 16 cm, 3 mm wide tip, angled laterally	1
<b>169-1520-04</b>	Sulcoplasty Bone File, 17 cm, 4 mm, slightly curved upwards	1
<b>169-1520-06</b>	Sulcoplasty Bone File, 17 cm, 6 mm, slightly curved upwards	1
<b>169-1562-02</b>	Sulcoplasty Osteotome, 16 cm, 2 mm wide tip, thickness 0.9mm	1
<b>169-1562-03</b>	Sulcoplasty Osteotome, 16 cm, 3 mm wide tip, thickness 0.9mm	1
<b>169-1562-04</b>	Sulcoplasty Osteotome, 16 cm, 4 mm wide tip, thickness 0.9mm	1
<b>169-1562-05</b>	Sulcoplasty Osteotome, 16 cm, 5 mm wide tip, thickness 0.9mm	1
<b>169-1562-06</b>	Sulcoplasty Osteotome, 16 cm, 6 mm wide tip, thickness 0.9mm	1
<b>169-1562-07</b>	Sulcoplasty Osteotome, 16 cm, 7 mm wide tip, thickness 0.9mm	1
<b>169-1562-08</b>	Sulcoplasty Osteotome, 16 cm, 8 mm wide tip, thickness 0.9mm	1
<b>169-1562-09</b>	Sulcoplasty Osteotome, 16 cm, 9 mm wide tip, thickness 0.9mm	1
<b>169-1562-10</b>	Sulcoplasty Osteotome, 16 cm, 10 mm wide tip, thickness 0.9mm	1
<b>169-1570-52</b>	Sulcoplasty / Osteotomy Bone Saw 17 cm, Cutting length 52mm, Cutting width 0.5mm	1
<b>169-1580-20</b>	Orthopedic hammer, length 200 mm, weight 225 g	1

## Orthopedic Hammer

## Sulcoplasty Instruments

### Sulcoplasty Scalpel Handle

No. 3, 16 cm, straight

**169-1500-03**



### Sulcoplasty Bone Lever

16 cm, 3 mm wide tip, angled laterally

**169-1537-03**



### Sulcoplasty Bone File



Product Code	Description
<b>169-1520-04</b>	17 cm, 4 mm, slightly curved upwards
<b>169-1520-06</b>	17 cm, 6 mm, slightly curved upwards

### Sulcoplasty Osteotome



Product Code	Description
<b>169-1562-02</b>	16 cm, 2 mm wide tip, thickness 0.9mm
<b>169-1562-03</b>	16 cm, 3 mm wide tip, thickness 0.9mm
<b>169-1562-04</b>	16 cm, 4 mm wide tip, thickness 0.9mm
<b>169-1562-05</b>	16 cm, 5 mm wide tip, thickness 0.9mm
<b>169-1562-06</b>	16 cm, 6 mm wide tip, thickness 0.9mm
<b>169-1562-07</b>	16 cm, 7 mm wide tip, thickness 0.9mm
<b>169-1562-08</b>	16 cm, 8 mm wide tip, thickness 0.9mm
<b>169-1562-09</b>	16 cm, 9 mm wide tip, thickness 0.9mm
<b>169-1562-10</b>	16 cm, 10 mm wide tip, thickness 0.9mm

### Sulcoplasty / Osteotomy Bone Saw

Cutting length 52mm, Cutting width 0.5mm

**169-1570-52**



### Orthopedic Hammer

Length 200 mm, Weight 225 g, blue silicone handle

**169-1580-20**



## STERILIZATION

Sterilization of products with fractional pre-vacuum procedure (in accordance with ISO 13060 / ISO 17665) in consideration of the respective national requirements. We recommend to perform a fractional pre-vacuum procedure with the following parameters:

- Fractional pre-vacuum (three times)
- Sterilization parameter 132 °C
- Holding period 3 min. (full cycle)
- Drying time 10 min.

## STORAGE

Sterilised products should be stored in a dry, clean and dust-free area at moderate temperature from 5°C to 40°C.

## ADDITIONAL INFORMATION

The user takes full responsibility for the processing facilities, the equipment and materials used, the personnel, as well as the proper execution of the processes to achieve the targeted results. This usually requires validation and routine monitoring of the process and equipment used.

## POWER TOOLS STERILIZATION

### *Cleaning, disinfection and sterilization guide*

#### Cleaning and disinfection

All consumables, parts and battery must be removed before cleaning. Always close the end cap of the battery chamber before cleaning!

Wipe the surfaces immediately after use with a lint-free cloth moistened with a cleaning agent or disinfectant, or use a disinfectant spray, to prevent exudates or other contamination from drying on the surface.

For this manual wipe-down, use a cleaning agent or disinfectant approved for surface disinfection under national regulations (DGHM – German Association of Hygiene and Microbiology). Please follow the manufacturer's instructions for correct dilution, exposure time etc.

In the case of heavy contamination, the power tool can also be carefully cleaned under running water (machine cleaning or soak cleaning is not permitted).

#### Note

Excessive exposure to saline solutions or solutions containing iodine or chloride may cause harmful reactions. Damage may also be caused by strong acids and alkaline solutions or incorrectly used disinfectants. The quality of the water used for cleaning and rinsing is another possible factor affecting corrosion or surface damage for the drill and attachments. The power tool must never be boiled or immersed in water or cleaning solutions.

#### **CAUTION!**

Always close the end cap of the battery chamber before cleaning!

Machine cleaning and ultrasonic cleaning in thermal disinfectors are not permitted!

#### Sterilization

The power tool with end cap of the battery chamber and funnel can be sterilised at up to 2 bar at 134°C / 273°F in the steam steriliser, for up to 6 minutes. Cooling time before use is 60 minutes.

It is advisable to place the equipment on a cloth or wrap it in a cloth to prevent external or internal damage. To ensure proper sterilisation, the battery chamber must always be closed.

#### Maintenance

The power tool should be regularly lubricated to ensure a long service life and smooth operation. We recommend the use of 1 drop Leilube special instrument oil.

#### **CAUTION!**

The rechargeable battery must never be sterilized.

# INSTRUCTIONS FOR USE OF SURGICAL INSTRUMENTS

## Warnings

The cleaning of narrow lumens or holes requires special attention! In general, our products will be delivered unsterile. All instruments have to be completely cleaned, disinfected and sterilized before initial use according to the following procedures.

## Indications

It is very important to check each surgical instrument for function and any visible damages before use. Damaged products should be scrapped or sent back to the manufacturer for maintenance. Restrictions of reprocessing: Frequent reprocessing has minimal effect on our instruments. The end of the product life cycle is determined by wear and damage through use.

Defective products should undergo the entire sterilization process before sending back to the manufacturer.

## Place of use

Immerse products in cold water immediately after each use (<40°C). Do not use cleaning agents or hot water (>40°C) as this may result in the fixation of residues and could reduce the cleaning success (risk of protein coagulation / denaturation). Remove surface contamination with a disposable, single-use towel or paper towel.

## Transport

Always store and transport instruments safely to avoid damages.

## Preparation for decontamination

When possible and where applicable, the instruments should be disassembled and/or unfastened or opened (e.g. for hinged instruments) before proceeding further with the processing steps.

### Manual Cleaning

- Immerse products in cold water for 5 min. and brush with a nylon brush thereafter.
- Flush products with a water pressure gun (with a static water pressure of at least 3.8 bar).
- Clean products in an ultrasonic bath with a smooth alkaline cleaner (neodisher Mediclean, Dr. Weigert, Hamburg).

### Machine Cleaning

Machine cleaning process (Program Vario TD ; G 7735 CD Miele):

- Pre-rinse for 2 min. with cold water
- Drain water
- Clean for 5 min. at 55°C with 0,5% alkaline cleaning agent (neodisher Mediclean, Dr. Weigert, Hamburg)
- Drain water
- Neutralize for 3 min. with cold tap water
- Drain water
- Rinse for 2 min. with cold tap water

Special manufacturer's instructions of the cleaning machine should be followed.

## Disinfection

### Manual Disinfection

1. Immerse products in disinfectant approved by RKI or VAH. Please follow the manufacturer's instructions for use of the disinfectant.
2. Rinse products with fully demineralized water.

### Automatic Disinfection

Automatic thermic disinfection in a cleaning and disinfection machine should conform to the national requirements to the A0-value.

### Drying

Manual drying should be carried out using a lint free cloth. The product should never be heated over 134°C. To avoid residual water in hollows, it is recommended to blow out with sterile compressed air.

Automatic drying should be in accordance to the automatic drying process of the cleaning and disinfection machine. If necessary, subsequent manual drying with lint free cloth and blowing out of lumen by sterile, oil-free compressed air may be done.

### Service, control and review

Test for function and check for contamination. If necessary, repeat the cleaning and disinfection process to remove residual contamination.

### Packaging

Products should be packaged in suitable sterile packaging.

## Contents

About Arthroscopy	166	Compression Bone Screws 4.0 - 6.0	147
Acetabulum Plate, standard	122	Compression Bone Screws - Combi Set	145
AO Quick-Connect Adapter	188	Compression Bone Screws Set - Medi/Maxi	147
Arthrodesis Plates, LeiLOX Locking, Titanium	94	Compression Bone Screws Set - Micro/Mini	146
Arthrodesis Plates, LeiLOX Locking, Stainless Steel	106	Compression Drill Guide	79
Arthrodesis Plates, standard	124	Cortical Screws (All)	126
Arthroscopes	173	Cortical Screws, LeiLOX Locking, Stainless Steel	108
Arthroscopes Equine	178	Cortical Screws, Non-Locking, Stainless Steel	110
Arthroscopy Rongeurs	179	Crimper	153
Arthroscopy Standard Instruments	172	Crimp Tubes	152
Arthroscopy Sterilization Storage System	174	Curette	177
Arthroscopy Trocar Set	173	Curved Hook Knife	176
Ball Head Burr	171	Depth Gauge (all)	201
Banana Knife	177	De Soutter hekaDrill	192
Battery Charger	189	De Soutter Rechargeable Drills	186
Bending Iron	112	Drill Bits (all)	199
Bending Irons AO Type (all)	201	Drill Bits, cannulated	149
Beta-Tricalcium Phosphate	164	Drill Guides (all)	199
Biopsy Spoon Forceps	169	Drill Guides for TTA Forks	40
Bone Awl	208	Drilling Machines	186
Bone Curette	207	Drills rechargeable	188
Bone Drills	80	Equine Arthroscopy Set	180
Bone File	207	Equine Dental Plugs	183
Bone Holding Forceps	202	Equine Dental Plug Set	182
Bone Lever	206	Forceps	203
Bone Packer	208	Gouge	207
Bone Plate Cutter	113	Grasping Forcep Alligator	169
Bone Plate DCP 1.5, 2.0, 2.4, 2.7	118	Guide Wires	137
Bone Plate Holding Forceps	113	hekaDrill Burs	193
Bone Plate Holding Forceps with Drill Guide	202	hekaDrill Console	192
Bone Plate Holding Retractor	113	hekaDrill Foot Pedal	193
Bone Plate Limited Contact	121	hekaDrill Handpiece and Attachment	192
Bone Plates Standard (all)	118	hekaDrill Irrigation Kit	193
Bone Reduction Forceps	203	Hook Grasping Forceps	178
Bone Substitutes	164	Hook Probe	171
Bone Tamper	208	Hook Probe	177
Bridge Plate, LeiLOX Locking, Stainless Steel	103	Hook Scissors	169
Cancellous Screws	129	Hydroxyapatitepaste Paste	164
Castroviejo	78	Instructions for Surgical Instruments	215
CBLO Locking Plates 2.0/2.4 Titanium	64	Instrument Cassette	210
CBLO Locking Plates 2.7/3.5 Titanium	66	Instruments, C-LOX	160
CBLO Rotation Chart	63	Instruments, C-LOX	161
CBLO Screws Locking & Non-Locking 2.0/2.4 Titanium	65	Instruments for LeiLOX Locking System	115
CBLO Screws Locking & Non-Locking 2.7/3.5 Titanium	67	Instruments (Micro)	206
CBLO Set 2.0/2.4 Titanium	64	Instruments TTA Standard	40
CBLO Set 2.7/3.5 Titanium	66	Jacobs Chuck	187
CBLO Surgery Protocol	62	Joseph Hook	208
CCWO Locking Plates 2.0/2.4 Titanium	72	Knives	171
CCWO Locking Plates 2.7/3.5 Titanium	74	K-Wire Instrument Set	135
CCWO Screws Locking & Non-Locking 2.0/2.4 Titanium	73	K-Wires	136
CCWO Screws Locking & Non-Locking 2.7/3.5 Titanium	75	K-Wire Set	134
CCWO Set 2.0/2.4 Titanium	72	Langenbeck Retractor	206
CCWO Set 2.7/3.5 Titanium	74	LeiCOM Application & Indications	144
CCWO Surgery Protocol	70	LeiCOM Surgical Technique	144
C-LOX Cages	158	LeiLOX Instruments	112
C-LOX Set	157	LeiLOX Instrument Set	112
C-LOX Surgical Protocol	156	LeiLOX Locking Plates 1.0 Titanium	85
C-LOX Templates	159	LeiLOX Locking Plates 1.5 Titanium	90
C-LOX Utilities	161	LeiLOX Locking Plates 2.0 Titanium	92
Compression Bone Screws 2.4 - 3.9	146	LeiLOX Locking Screws 1.5 Titanium	91
Compression Bone Screws 2.4 - 6.0	145	LeiLOX Locking Screws 2.0 Titanium	93

LeiLOX Locking Screws Stainless Steel	132	Senn Miller Hook	209
LeiLOX Locking Screws Titanium	131	S.O.S. Screw Removal	196
LeiLOX Locking Set 1.0/1.3 Titanium	84	Spinal	159
LeiLOX Locking Set 1.5/2.0 Titanium	88	Steinmann Pins	137
LeiLOX Locking Set 1.5 Titanium	89	Sterilization Container	204
LeiLOX Locking Set 2.0 Titanium	89	Sterilization Tray for Power Tools	191
LeiLOX Set, Arthrodesis 2.0-3.5	99	Straight Plate, LeiLOX Locking, Stainless Steel	102
LeiLOX Sets, Reconstruction 2.0/2.4 + 2.7/3.5	100	Sulcoplasty Instruments	213
LeiLOX Sets, Straight + Reconstruction	101	Sulcoplasty Set	212
LeiLOX Sets, Straight Plates 2.0/2.4 + 2.7/3.5	98	Suture Anchor	152
LeiLOX Sets, Straight Plates 2.0/2.4 + 2.7/3.5	99	Sutures	153
LeiMESH 3D Dynamic Mesh Set	140	Tensioning Device	153
LeiMESH Cuttable Mesh Titanium	141	Tibia Tappet	22
LeiMESH System Instruments	141	Tibia Tappet for TPLO Patella Luxation	58
Limited Contact DCP Plate	121	Torque Limiting Screwdriver Handle	80
Locking Drill Guides (all)	200	T-Plate, LeiLOX Locking, Stainless Steel	105
Locking Plug, LeiLOX	109	T-Plate (Phillips, T-shape)	124
Locking Screws (All)	130	T-Plate, standard	123
L-Plate, standard	123	TPLO / CBLO / CCWO Instrument Set	78
Mini Lambotte Osteotome	174	TPLO Jig	78
Neuro-Surgery	158	TPLO Locking Plates 2.0/2.4 Stainless Steel	48
Non-Locking Cortical Screws (All)	127	TPLO Locking Plates 2.7/3.5 Stainless Steel	50
Orthopedic Cerclage	135	TPLO & Patella Luxation	59
Orthopedic Hammer	213	TPLO Patella Luxation Spacers	58
Osteotome	210	TPLO Rotation Chart	46
Patella Luxation	30	TPLO Saw Adapter	187
Patella Luxation Spacers	22	TPLO Saw Blades	191
Patella Luxation & TTA	21	TPLO Screws 2.0/2.4 Stainless Steel	49
Patella Saw	22	TPLO Screws 2.0/2.4 Titanium	55
Patella Saw	32	TPLO Screws 2.7/3.5 Stainless Steel	51
Periosteal Elevator	177	TPLO Screws 2.7/3.5 Titanium	57
Periosteal Elevator	206	TPLO Set 2.0/2.4 Stainless Steel	48
Pick Probe	177	TPLO Set 2.7/3.5 Stainless Steel	50
Pin Driver	187	TPLO Surgery Protocol	44
Plate Holding Forceps	24	TPLO Swing Locking Plates 2.0/2.4 Titanium	54
Plates (all)	119	TPLO Swing Locking Plates 2.7/3.5 Titanium	56
Power Tools Sterilization	214	TPLO Swing Set 2.0/2.4 Titanium	54
Radiography Calibration Ball	81	TPLO Swing Set 2.7/3.5 Titanium	56
RAPID Luxation Instruments	33	TPLO Weight Guide	47
RAPID Luxation Plates	30	TTA Cages	37
RAPID Luxation Saw Guide	32	TTA Cuttable Cages	37
RAPID Luxation Screws	31	TTA ESY Set	36
RAPID Luxation Set	29	TTA RAPID® Studies	13
RAPID Luxation Surgery Protocol	28	TTA RAPID® Surgery Protocol	12
Rechargeable Batteries	189	TTA RAPID® Technique	10
Reconstruction Plate, LeiLOX Locking, Stainless Steel	104	TTA RAPID Giant Cages	19
Reconstruction Plate, straight/curved, standard	122	TTA RAPID Implants	18
Retractor	209	TTA RAPID Instruments	23
Rinse Cannula Set	174	TTA RAPID Instrument Set	16
Sagittal Saw Adapter	187	TTA RAPID Saw Guide	23
Saw Blades (all)	190	TTA RAPID Screws	20
Scalpel Handle	209	TTA RAPID Sets	14
Screw Depth Gauge, cannulated	148	TTA RAPID Spreader	23
Screwdriver Handles (all)	198	TTA RAPID Tiny Cages	18
Screwdriver Shaft (all)	200	TTA Screws	38
Screwdriver Shaft, cannulated	148	TTA Spacers	38
Screwdriver Shafts for Dental Plugs	183	TTA Standard Plates	37
Screwdriver T-Handle	184	TTA Standard Set	36
Screw Head Countersink, cannulated	149	Twist Drill	25
Screw Racks (all)	198	Van Ryssen Arthroscopy Set	167
Screw Removal Set S.O.S.	196	Van Ryssen Series	168
Screws (C-LOX)	160	VAN RYSSSEN Signature Series	170
Screws for RAPID Luxation	31	Washers	128
Screws for TTA RAPID	20	X-Ray Markers	210

## Product Code Index

11-0966-14TC ....141	125-5006-00.... 186	128-0940-24 .... 200	130-11-2007.....121	130-1848-20 .....118
17-3105-08.....78	125-5006-00.... 188	128-0940-25 .....41	130-11-2008.....121	130-1863-09 .....123
23-1005-20 .....22	125-5006-00....189	128-0940-25 .... 200	130-11-2009.....121	130-1864-09 .....123
23-1005-20 .....32	125-5007-00 ....189	128-1013-00 .....116	130-11-2010.....121	130-5215-10.....128
23-1005-90 .....22	125-5008-00 ....189	128-1013-00 .... 200	130-11-2020.....121	130-6252-12 .....128
23-1005-90 .....32	125-5020-00 .... 186	128-1520-15.....25	130-11-6004 .....118	130-7324-14.....128
23-1363-14.....135	125-5050-00 .... 188	128-1520-15.....116	130-11-6005 .....118	130-8327-16 .....128
23-1364-14.....135	125-5050-10 ....191	128-1520-15.....196	130-11-6006 .....118	130-9435-16 .....128
23-3513-00 .....135	125-5051-00 .... 188	128-1520-15.....200	130-11-6007 .....118	131-20-0304 .....124
23-3805-12 .....174	125-5052-00 .... 188	128-1520-20.....25	130-11-6008 .....118	131-20-0305 .....124
23-3806-12 .....174	125-5053-00 .... 188	128-1520-20.....33	130-11-6009 .....118	131-20-0306 .....124
23-3807-12.....174	125-5054-00 .... 188	128-1520-20.....41	130-11-6010.....118	131-35-0404 .....124
23-5535-18T .....135	125-5055-00 .... 186	128-1520-20.....116	130-11-6011.....118	131-35-0406 .....124
23-5795-22T .....135	125-5055-00 .... 186	128-1520-20.... 200	130-11-6012.....118	131-35-0505 .....124
23-5865-24T .....113	125-5055-00 .... 188	128-1600-00 ....141	130-11-6013.....118	131-35-0506 .....124
24-4310-17.....153	125-5055-00 ....189	128-2024-08 .....25	130-11-6014.....118	131-35-0508 .....124
100-0000-02.....210	125-5056-00 ....189	128-2024-08 .....33	130-12-0103.....123	132-0003-08.....18
100-2000-25 .....81	125-5057-00 ....189	128-2024-08 .....80	130-12-0203.....123	132-0003-10 .....18
102-1210-25.....190	125-5059-00 ....189	128-2024-08 .....116	130-12-0604 .....122	132-0003-13 .....18
102-1211-30.....190	125-6050-00.....192	128-2024-08 .... 200	130-12-0605 .....122	132-0003-16 .....18
102-1212-25.....190	125-6051-00 .....192	128-2418-24.....79	130-12-0606 .....122	132-0006-13 .....18
102-1213-25.....190	125-6052-00 .....192	128-2418-24.....199	130-30-0004.....120	132-0006-16 .....18
102-1411-27.....190	125-6052-01 .....192	128-2431-06 .... 148	130-30-0005.....120	132-0006-19 .....18
102-1411-35.....190	125-6053-00 .....193	128-2431-06 .... 201	130-30-0006.....120	132-0006-22 .....18
102-1414-42.....190	125-6053-01 .....193	128-2431-31.....149	130-30-0007.....120	132-0009-16 .....19
102-1420-50.....190	125-6054-00 .....193	128-2535-35 .....79	130-30-0008.....120	132-0009-19 .....19
102-1511-27.....190	128-0122-25 .....141	128-2535-35 .....199	130-30-0009.....120	132-0009-22 .....19
102-1511-35.....190	128-0300-15 .....196	128-2720-27 .....79	130-30-0010.....120	132-0009-25 .....19
102-1514-42.....190	128-0525-21 .....24	128-2720-27 .....199	130-30-0011 .....120	132-0012-19.....19
102-1520-50.....190	128-0525-21 .....41	128-2735-10.....25	130-30-0012 .....120	132-0012-22.....19
102-1611-27.....190	128-0525-21 .... 203	128-2735-10.....41	130-30-0013 .....120	132-0012-25.....19
102-1611-35.....190	128-0537-10.....113	128-2735-10.....80	130-30-0014 .....120	132-0012-28.....19
102-1614-42.....190	128-0538-13 .....113	128-2735-10.....116	130-30-0015 .....120	132-0015-19.....19
102-1620-50 .....190	128-0538-13 .... 202	128-2735-10.... 200	130-30-0016 .....120	132-0015-22 .....19
102-1711-27.....190	128-0539-13 .....113	128-3039-08 .... 148	130-30-0018 .....120	132-0015-25 .....19
102-1711-35.....190	128-0539-13 .....202	128-3039-08 ....201	130-30-0020.....120	132-0015-28 .....19
102-1714-42.....190	128-0540-14 .... 202	128-3039-39 .....149	130-30-0022.....120	132-0018-22 .....19
102-1912-40.....190	128-0540-15 .... 202	128-4050-10 .... 148	130-30-0024.....120	132-0018-25 .....19
102-1916-40 .....190	128-0540-16 .... 202	128-4050-10 ....201	130-31-0005 .....120	132-0018-28 .....19
102-2026-18.....190	128-0541-09 .... 203	128-4050-50 .....149	130-31-0006.....120	132-0018-31 .....19
102-2026-24.....190	128-0541-14..... 203	128-4354-00.....78	130-31-0007 .....120	132-0023-08.....18
102-2100-09 .....191	128-0543-13 .... 203	128-4355-00.....78	130-31-0008.....120	132-0023-10.....18
102-2100-12.....191	128-0544-03 .... 202	128-4356-00.....78	130-31-0009.....120	132-0023-13.....18
102-2100-15.....191	128-0544-07 .... 202	128-5060-15 .... 148	130-31-0010 .....120	132-0026-09.....18
102-2100-18.....191	128-0803-00.....141	128-5060-15 ....201	130-31-0011 .....120	132-0026-11 .....18
102-2100-21.....191	128-0807-00 .....198	128-5060-60.....149	130-31-0012 .....120	132-0026-13 .....18
102-2100-24.....191	128-0820-24 .....112	129-0051-23 .....153	130-31-0013 .....120	132-0045-09.....18
102-2100-27.....191	128-0827-35 .....112	130-11-0302.....123	130-31-0014 .....120	132-0045-12 .....18
102-2100-30 .....191	128-0880-27 .....201	130-11-0339.....123	130-31-0015 .....120	132-0045-15 .....18
102-2100-33 .....191	128-0881-15 .....112	130-11-0349 .....123	130-31-0016 .....120	132-0045-18 .....18
102-16506-27 ....190	128-0881-15 .....201	130-11-0402 .....123	130-31-0018 .....120	132-0075-13 .....18
102-16510-25 ....190	128-0881-27 .....201	130-11-0502.....123	130-31-0020 .....120	132-0075-16 .....18
102-16515-46 .....190	128-0900-15 .....25	130-11-0606 .....122	130-31-0022 .....120	132-0075-19 .....18
102-16520-50 .....190	128-0900-15 .....33	130-11-1014 .....118	130-31-0024 .....120	132-0075-22 .....18
111-0015-10.....134	128-0900-15 .... 200	130-11-1015 .....118	130-50-0106 .....122	132-0105-16.....19
111-0015-20.....135	128-0900-20 .....25	130-11-1016.....118	130-50-0108 .....122	132-0105-19.....19
111-0016-00 .....167	128-0900-20 .....33	130-11-1017.....118	130-50-0110 .....122	132-0105-22 .....19
123-1019-00 .....182	128-0900-20 .....41	130-11-1018.....118	130-50-0112 .....122	132-0105-25 .....19
123-3019-00 .....182	128-0900-20 .... 200	130-11-1019.....118	130-50-0114 .....122	132-0135-19.....19
125-5000-00.... 186	128-0900-25 .....41	130-11-1020.....118	130-50-0116 .....122	132-0135-22.....19
125-5000-10 .....191	128-0900-25 .... 200	130-11-1021.....118	130-1848-04.....118	132-0135-25.....19
125-5001-00 .....187	128-0905-15 .....198	130-11-1022.....118	130-1848-05.....118	132-0135-28.....19
125-5002-00 .....187	128-0905-17 ....198	130-11-1420.....122	130-1848-06 .....118	132-0152-06 .....18
125-5003-00 .....187	128-0911-25.....198	130-11-2004.....121	130-1848-07 .....118	132-0152-08 .....18
125-5004-00 .....187	128-0940-24 .....25	130-11-2005.....121	130-1848-08 .....118	132-0152-10.....18
125-5005-00 .....187	128-0940-24 .....33	130-11-2006.....121	130-1848-09.....118	132-0153-07 .....18
125-5006-00.... 186	128-0940-24 .....41		130-1848-10 .....118	132-0153-09 .....18

132-0153-11.....18	132-8020-03L ....30	140-12-0007 .....118	140-50-0012 .....122	142-0215-658 .....90
132-0165-22 .....19	132-8020-03R.....22	140-12-0008 .....118	140-50-0014 .....122	142-0215-805 .....90
132-0165-25 .....19	132-8020-03R.....30	140-12-0009 .....118	140-50-0016 .....122	142-0215-809 .....90
132-0165-28 .....19	132-8020-04L.....22	140-12-0010 .....118	140-50-0018 .....122	142-0215-925L .....90
132-0165-31.....19	132-8020-04L.....30	140-12-0011.....118	140-50-0020.....122	142-0215-925R...90
132-0245-08 .....18	132-8020-04R.....22	140-12-0012 .....118	140-50-0022.....122	142-0215-950L...90
132-0245-10.....18	132-8020-04R.....30	140-12-0013 .....118	140-0620-24.....123	142-0215-950R...90
132-0245-12.....18	132-8030-01L.....22	140-12-0014 .....118	140-0620-25.....123	142-0220-04.....92
132-4000-13 .....23	132-8030-01L.....30	140-13-2004 .....121	140-0620-26.....123	142-0220-4H.....93
132-4010-13.....23	132-8030-01R...22	140-13-2005 .....121	140-0620-27.....123	142-0220-05.....92
132-4015-13.....23	132-8030-01R...30	140-13-2006 .....121	140-0620-28.....123	142-0220-06.....92
132-4020-00.....24	132-8030-02L.....22	140-13-2007 .....121	140-1011-00.....164	142-0220-07.....92
132-4020-00.....41	132-8030-02L...30	140-13-2008 .....121	140-2011-00...164	142-0220-08.....92
132-4030-10 .....23	132-8030-02R.....22	140-13-2009 .....121	141-9090-10 ....140	142-0220-09.....92
132-4030-10 .....32	132-8030-02R.....30	140-13-2010.....121	141-9090-15 .....141	142-0220-10.....92
132-4040-00.....23	132-8030-03L.....22	140-13-2011.....121	141-9091-10.....140	142-0220-10Z.....93
132-4040-00.....32	132-8030-03L.....30	140-13-2012.....121	142-0100-01.....78	142-0220-20.....92
132-4041-00.....23	132-8030-03R.....22	140-13-2013.....121	142-0100-02.....50	142-0220-38.....92
132-4041-00.....32	132-8030-03R.....30	140-13-2014.....121	142-0100-10.....50	142-0220-49.....92
132-4042-00.....23	132-8030-04L.....22	140-20-0002.....119	142-0100-20.....78	142-0220-60.....94
132-4042-00.....32	132-8030-04L.....30	140-20-0004.....119	142-0150-00.....48	142-0220-68.....94
132-4070-00.....22	132-8030-04R.....22	140-20-0005.....119	142-0210-04.....84	142-0220-410....93
132-4070-00.....32	132-8030-04R.....30	140-20-0006.....119	142-0210-4H.....85	142-0220-504L...92
132-4071-00.....22	132-8200-01 .....30	140-20-0007.....119	142-0210-05.....84	142-0220-504R...92
132-4071-00.....32	132-8200-02 .....30	140-20-0008.....119	142-0210-06.....84	142-0220-618.....92
132-4080-12 .....23	132-8200-03 .....30	140-20-0009.....119	142-0210-07.....84	142-0220-627.....92
132-4080-16 .....23	132-9025-00 ....164	140-20-0010.....119	142-0210-08.....84	142-0220-636.....92
132-4080-16 .....41	134-0100-01 .....157	140-20-0011.....119	142-0210-09.....84	142-0220-648.....92
132-5000-00/A....14	134-0144-08 .....158	140-20-0012.....119	142-0210-10.....84	142-0220-668.....92
132-5000-00/A....15	134-0146-08 .....158	140-20-0013.....119	142-0210-20.....84	142-0220-805.....92
132-5000-00/A....15	134-0164-08 .....158	140-20-0014.....119	142-0210-38.....84	142-0220-809.....92
132-5000-00/A....15	134-0165-10 .....158	140-20-0015.....119	142-0210-49.....84	142-0220-925L...92
132-5000-00/A....16	134-0166-08 .....158	140-20-0016.....119	142-0210-453....85	142-0220-925R...92
132-5000-10/A....16	134-0167-10.....158	140-20-0017.....119	142-0210-504L...84	142-0220-950L...92
132-6000-10 .....16	134-0185-10 .....158	140-20-0018.....119	142-0210-504R...84	142-0220-950R...92
132-6002-00 .....14	134-0187-10.....158	140-20-2004 .....121	142-0210-610....84	142-1013-00.....84
132-6003-00 .....15	134-0206-12 .....158	140-20-2005 .....121	142-0210-615....84	142-1013-10.....84
132-6004-00.....15	134-0208-12 .....158	140-20-2006 .....121	142-0210-625....84	142-1120-00.....48
132-6005-00.....15	134-0500-01 .....157	140-20-2007 .....121	142-0210-633....84	142-1120-10.....48
132-6006-00.....16	134-0700-22 .....161	140-20-2008 .....121	142-0210-643....84	142-1124-00.....48
132-6010-00 .....16	134-0750-16 .....161	140-20-2009 .....121	142-0210-809....85	142-1124-10.....48
132-6012-00 .....14	134-0750-20 .....161	140-20-2010 .....121	142-0210-925L...85	142-1127-00.....50
132-6013-00 .....15	134-0750-22 .....161	140-20-2011 .....121	142-0210-925R...85	142-1127-10.....50
132-6014-00 .....15	134-0800-27 ....160	140-20-2012 .....121	142-0210-950L...85	142-1135-00.....50
132-6015-00 .....15	134-0800-27 ....200	140-20-2014 .....121	142-0210-950R...85	142-1135-10.....50
132-6016-00 .....16	134-0900-24 ....200	140-24-0004.....119	142-0215-04.....90	142-1135-50.....50
132-6200-00.....14	134-9144-08 .....159	140-24-0005.....119	142-0215-4H.....91	142-1135-60.....50
132-6200-10.....14	134-9146-08 .....159	140-24-0006.....119	142-0215-05.....90	142-1500-00.....89
132-6500-00.....17	134-9164-08 .....159	140-24-0007.....119	142-0215-06.....90	142-1500-10.....89
132-6500-10.....17	134-9165-10 .....159	140-24-0008.....119	142-0215-07.....90	142-1520-00.....88
132-8000-00.....29	134-9166-08 .....159	140-24-0009.....119	142-0215-08.....90	142-1520-10.....88
132-8000-01.....29	134-9167-10.....159	140-24-0010.....119	142-0215-09.....90	142-1520-50.....88
132-8000-10.....29	134-9185-10 .....159	140-24-0011.....119	142-0215-10.....90	142-1520-60.....88
132-8010-02L....22	134-9187-10.....159	140-24-0012.....119	142-0215-10Z....91	142-2000-00.....89
132-8010-02L....30	134-9206-12 .....159	140-24-0013.....119	142-0215-20.....90	142-2000-10.....89
132-8010-02R....22	134-9208-12 .....159	140-24-0014.....119	142-0215-38.....90	142-2020-00.....101
132-8010-02R....30	140-05-1168 .....124	140-24-0015.....119	142-0215-49.....90	142-2020-01.....101
132-8010-04L....22	140-05-1169 .....124	140-24-0016.....119	142-0215-55.....94	142-2020-60....106
132-8010-04L....30	140-05-1170 .....124	140-24-0017.....119	142-0215-60.....94	142-2024-00.....98
132-8010-04R....22	140-05-1171 .....124	140-24-0018.....119	142-0215-120L...94	142-2024-01.....98
132-8010-04R....30	140-05-1172 .....124	140-24-0019.....119	142-0215-120R...94	142-2024-50.....112
132-8010-06L....22	140-05-1173 .....124	140-24-0020.....119	142-0215-135L...94	142-2024-51.....112
132-8010-06L....30	140-05-1174.....124	140-50-0004.....122	142-0215-135R...94	142-2024-60.....99
132-8010-06R....22	140-05-1175.....124	140-50-0005.....122	142-0215-475....91	142-2024-62.....99
132-8010-06R....30	140-05-1177 .....124	140-50-0006.....122	142-0215-504L...90	142-2024-70.....106
132-8020-02L....22	140-06-1176 .....124	140-50-0007.....122	142-0215-504R...90	142-2024-90....100
132-8020-02L....30	140-06-1178 .....124	140-50-0008.....122	142-0215-614....90	142-2024-91....100
132-8020-02R....22	140-12-0004 .....118	140-50-0009.....122	142-0215-621....90	142-2024-120L...107
132-8020-02R....30	140-12-0005 .....118	140-50-0010.....122	142-0215-635....90	142-2024-120R...107
132-8020-03L....22	140-12-0006 .....118	140-50-0011.....122	142-0215-645....90	142-2024-135L...107

142-2024-135R ...107	142-3020-20 .....102	142-3127-12 ..... 104	142-4135-18.....103	144-1018-25 .....136
142-2027-80 .... 106	142-3024-04 .....102	142-3127-14..... 104	142-4135-20.....103	144-1018-30 .....136
142-2027-90..... 106	142-3024-05 .....102	142-3127-16..... 104	142-4200-00..... 64	144-1020-10 .....79
142-2027-120L...107	142-3024-06 .....102	142-3127-18..... 104	142-4200-10..... 64	144-1020-10 .....116
142-2027-120R ...107	142-3024-07 .....102	142-3127-20..... 104	142-8020-00.....58	144-1020-10 .....134
142-2027-135L...107	142-3024-08 .....102	142-3135-04 .... 104	142-8024-00.....58	144-1020-10 .....136
142-2027-135R ...107	142-3024-09 .....102	142-3135-05 .... 104	142-8027-00.....58	144-1020-15.....134
142-2320-00 ..... 64	142-3024-10.....102	142-3135-06 .... 104	142-8035-00.....58	144-1020-15.....136
142-2320-10..... 64	142-3024-12.....102	142-3135-07..... 104	142-8035-10..... 58	144-1020-20 .....134
142-2324-00 ..... 64	142-3024-14.....102	142-3135-08 .... 104	143-0001-10 .....152	144-1020-20 .....136
142-2324-10..... 64	142-3024-16.....102	142-3135-09 ..... 104	143-0001-12 .....152	144-1020-25 .....136
142-2327-00 .....66	142-3024-18.....102	142-3135-10..... 104	143-0001-14 .....152	144-1020-30 .....136
142-2327-10..... 66	142-3024-20 .....102	142-3135-12..... 104	143-0008-50 .....153	144-1025-10 .....24
142-2335-00 ..... 66	142-3027-04 .....102	142-3135-14..... 104	143-0008-80 .....153	144-1025-10 .....33
142-2335-10..... 66	142-3027-05 .....102	142-3135-16..... 104	143-0008-100.....153	144-1025-10 .....79
142-2335-50 ..... 66	142-3027-06 .....102	142-3135-18..... 104	143-0010-50 .....153	144-1025-10 .....116
142-2335-60 ..... 66	142-3027-07 .....102	142-3135-20..... 104	143-0010-80 .....153	144-1025-10 .....134
142-2424-00 .... 101	142-3027-08 .....102	142-3200-00 .....99	143-0010-100 ....153	144-1025-10 .....136
142-2424-01 .....101	142-3027-09 .....102	142-3200-10 .....99	143-1000-02 .....135	144-1025-15.....134
142-2727-00 .....101	142-3027-10.....102	142-3300-00 .....99	143-1000-03 .....135	144-1025-15.....136
142-2727-01.....101	142-3027-12.....102	142-3300-10 .....99	143-1000-04 .....134	144-1025-20 .....134
142-2725-115... 106	142-3027-14.....102	142-3535-140 ... 106	143-1000-04 .....135	144-1025-20 .....136
142-2735-135L ...107	142-3027-16.....102	142-3620-35 .....105	143-1000-05 .....135	144-1025-25 .....136
142-2735-135R ...107	142-3027-18.....102	142-3620-37 .....105	143-1000-06 .....134	144-1025-30 .....136
142-2800-10 .....48	142-3027-20.....102	142-3624-35 .....105	143-1000-06 .....135	144-1030-10 .....79
142-2800-10 .....54	142-3035-04 .....102	142-3624-37 .....105	143-1000-07 .....135	144-1030-10 .....116
142-2800-20 .....56	142-3035-05 .....102	142-3627-35.....105	143-1000-08 .....134	144-1030-10 .....136
142-2820-00 .....54	142-3035-06 .....102	142-3627-37.....105	143-1000-08 .....135	144-1030-15 .....136
142-2820-10.....54	142-3035-07 .....102	142-3635-35 .....105	143-1000-09 .....135	144-1030-20 .....136
142-2820-24 .....54	142-3035-08 .....102	142-3635-37 .....105	143-1000-10 .....134	144-1030-25 .....136
142-2824-00 .....54	142-3035-09 .....102	142-4000-01 .....66	143-1000-10 .....135	144-1030-30 .....136
142-2824-10.....54	142-3035-10.....102	142-4000-10 .....66	143-1000-12.....135	144-1035-10.....136
142-2827-00 .....56	142-3035-12.....102	142-4120-08 .....103	143-1000-15 .....135	144-1035-15.....136
142-2827-10.....56	142-3035-14.....102	142-4120-09 .....103	144-1008-10 .....136	144-1035-20 .....136
142-2827-35.....56	142-3035-16.....102	142-4120-10.....103	144-1008-15 .....136	144-1035-25 .....136
142-2835-00 .....56	142-3035-18.....102	142-4120-11.....103	144-1008-20 .....136	144-1035-30 .....136
142-2835-10.....56	142-3035-20 .....102	142-4120-12.....103	144-1009-15 .... 148	144-1040-10 .....136
142-2835-50 .....56	142-3100-00 .... 100	142-4120-13.....103	144-1010-10.....79	144-1040-15 .....136
142-2835-60 .....56	142-3100-02 .... 100	142-4120-14.....103	144-1010-10.....116	144-1040-20 .....136
142-2890-00 .....58	142-3120-04 .... 104	142-4120-16.....103	144-1010-10.....134	144-1040-25 .....136
142-2891-00 .....58	142-3120-05 .... 104	142-4120-18.....103	144-1010-10.....136	144-1040-30 .....136
142-2900-10 .....72	142-3120-06 .... 104	142-4120-20.....103	144-1010-15.....134	144-1045-15 .....136
142-2900-20 .....74	142-3120-07 .... 104	142-4124-08 .....103	144-1010-15.....136	144-1045-20 .....136
142-2920-00 .....72	142-3120-08 .... 104	142-4124-09 .....103	144-1010-20 .....134	144-1045-25 .....136
142-2920-10.....72	142-3120-09 .... 104	142-4124-10.....103	144-1010-30 .....136	144-1045-30 .....136
142-2920-24.....72	142-3120-10..... 104	142-4124-11.....103	144-1012-10.....136	144-1050-15 .....136
142-2924-00 .....72	142-3120-12..... 104	142-4124-12.....103	144-1012-15.....136	144-1050-20 .....136
142-2924-10.....72	142-3120-14..... 104	142-4124-13.....103	144-1012-20.....136	144-1050-25 .....136
142-2927-00 .....74	142-3120-16..... 104	142-4124-14.....103	144-1014-10.....136	144-1050-30 .....136
142-2927-10.....74	142-3120-18..... 104	142-4124-16.....103	144-1014-15.....136	144-1060-15 .....136
142-2927-35.....74	142-3120-20..... 104	142-4124-18.....103	144-1014-20.....136	144-1060-20 .....136
142-2935-00 .....74	142-3124-04 .... 104	142-4124-20.....103	144-1015-10.....24	144-1060-25 .....136
142-2935-10.....74	142-3124-05 .... 104	142-4127-08 .... 103	144-1015-10.....33	144-1060-30 .....136
142-2935-50 .....74	142-3124-06 .... 104	142-4127-09.....103	144-1015-10.....134	144-1510-10.....136
142-2935-60 .....74	142-3124-07..... 104	142-4127-10.....103	144-1015-10.....136	144-1510-15.....136
142-3000-00.....98	142-3124-08 .... 104	142-4127-11 .....103	144-1015-15.....134	144-1510-20.....136
142-3010-00.....112	142-3124-09 .... 104	142-4127-12 .....103	144-1015-15.....136	144-1510-25 .....136
142-3010-01 .....112	142-3124-10..... 104	142-4127-13 .....103	144-1015-15.....148	144-1510-30 .....136
142-3010-02 .....98	142-3124-12..... 104	142-4127-14 .....103	144-1015-20.....134	144-1512-10.....136
142-3020-04 .....102	142-3124-14..... 104	142-4127-16.....103	144-1015-20.....136	144-1512-15 .....136
142-3020-05 .....102	142-3124-16..... 104	142-4127-18.....103	144-1015-25.....136	144-1512-20.....136
142-3020-06 .....102	142-3124-18..... 104	142-4127-20.....103	144-1015-30 .....136	144-1512-25 .....136
142-3020-07 .....102	142-3124-20..... 104	142-4135-08 .....103	144-1016-10.....136	144-1512-30.....136
142-3020-08 .....102	142-3127-04..... 104	142-4135-09 .....103	144-1016-15.....136	144-1514-10.....136
142-3020-09 .....102	142-3127-05..... 104	142-4135-10.....103	144-1016-20 .....136	144-1514-15.....136
142-3020-10.....102	142-3127-06..... 104	142-4135-11 .....103	144-1016-25 .....136	144-1514-20.....136
142-3020-12.....102	142-3127-07..... 104	142-4135-12.....103	144-1016-30 .....136	144-1514-25.....136
142-3020-14.....102	142-3127-08..... 104	142-4135-13.....103	144-1018-10.....136	144-1514-30 .....136
142-3020-16.....102	142-3127-09..... 104	142-4135-14.....103	144-1018-15.....136	144-1515-10.....136
142-3020-18.....102	142-3127-10..... 104	142-4135-16.....103	144-1018-20.....136	144-1515-15.....136

144-1515-20.....136	144-2015-30 .....137	148-0080-20.....80	150-0520-00.....198	163-600-10 .....177
144-1515-25.....136	144-2016-10 .....137	148-0080-20.....114	150-0524-00.....198	163-600-11 .....177
144-1515-30.....136	144-2016-15.....137	148-0080-20.....199	150-0527-00.....198	163-600-12 .....177
144-1516-10.....136	144-2016-20 .....137	148-0080-25.....40	150-0535-00.....198	163-600-13 .....177
144-1516-15.....136	144-2016-25 .....137	148-0080-25.....80	150-0863-00.....196	163-600-14 .....177
144-1516-15.....137	144-2016-30 .....137	148-0080-25.....199	150-0864-00.....196	163-600-15 .....177
144-1516-20.....136	144-2018-10.....137	148-0080-27.....199	150-0865-00.....134	163-600-16 .....177
144-1516-20.....137	144-2018-15.....137	148-0080-30.....199	150-0866-00.....135	163-600-17 .....177
144-1516-25.....136	144-2018-20 .....137	148-0080-32.....199	150-4027-00.....198	163-600-18 .....177
144-1516-25.....137	144-2018-25 .....137	148-0080-35.....199	150-4035-00.....198	163-600-19 .....177
144-1516-30 .....136	144-2018-30 .....137	148-0080-45.....199	150-5401-00.... 204	163-600-20 .....177
144-1516-30 .....137	144-2020-10 .....137	148-0081-07.....114	150-5401-30.... 204	163-600-21 .....177
144-1518-10.....136	144-2020-15 .....137	148-0081-07.....199	150-5402-00.... 204	163-600-22 .....177
144-1518-15.....136	144-2020-20 .....137	148-0081-10 .....114	150-5402-30.... 204	163-1000-00.... 180
144-1518-15.....137	144-2020-25 .....137	148-0081-10 .....199	160-2401-00.....172	164-0010-00.....115
144-1518-20.....136	144-2020-30 .....137	148-0081-11 .....25	160-2402-00.....172	164-0010-00.... 200
144-1518-20.....137	144-2025-10 .....137	148-0081-11 .....114	160-2408-00.....172	164-0013-00.....115
144-1518-25.....136	144-2025-15 .....137	148-0081-11 .....199	160-2413-00.....172	164-0013-00.... 200
144-1518-25.....137	144-2025-20 .....137	148-0081-15 .....25	160-2420-00.....172	164-0015-00.....115
144-1518-30 .....136	144-2025-25 .....137	148-0081-15 .....33	160-2421-00.....172	164-0015-00.... 200
144-1518-30 .....137	144-2025-30 .....137	148-0081-15 .....80	162-0013-30.....173	164-0020-00.....115
144-1520-10.....136	144-2030-10 .....137	148-0081-15 .....114	162-0016-30.....173	164-0020-00.... 200
144-1520-15.....136	144-2030-15 .....137	148-0081-15 .....199	162-0017-30.....173	164-0027-10.....161
144-1520-15.....137	144-2030-20 .....137	148-0081-18 .....25	162-0018-30.....173	164-0027-12.....161
144-1520-20 .....136	144-2030-25 .....137	148-0081-18 .....33	162-0019-00.....178	164-0027-14.....161
144-1520-20 .....137	144-2030-30 .....137	148-0081-18 .....40	162-0019-30.....178	164-0027-16.....161
144-1520-25 .....136	144-2035-15 .....137	148-0081-18 .....80	162-0021-20.....173	164-0027-18.....161
144-1520-25 .....137	144-2035-20 .....137	148-0081-18 .....114	162-0021-30.....173	164-0027-20.....161
144-1520-30 .....136	144-2035-25 .....137	148-0081-18 .....199	162-0021-45.....173	164-0050-09.....24
144-1520-30 .....137	144-2035-30 .....137	148-0081-20 .....25	162-0031-65.....173	164-0050-09.....32
144-1525-10.....137	144-2040-15 .....137	148-0081-20 .....40	162-0035-03.....173	164-0050-09.... 201
144-1525-15.....137	144-2040-20 .....137	148-0081-20 .....80	162-0035-14.....173	164-0050-16.....24
144-1525-20 .....137	144-2040-25 .....137	148-0081-20 .....114	162-0035-18.....173	164-0050-16.....41
144-1525-25 .....137	144-2040-30 .....137	148-0081-20 .....161	162-0035-22.....173	164-0051-17.....201
144-1525-30 .....137	144-2045-15 .....137	148-0081-20 .....199	162-0036-03.....173	164-0070-18.....24
144-1530-10 .....137	144-2045-20 .....137	148-0081-25 .....40	162-0036-14.....173	164-0070-18.....33
144-1530-15.....137	144-2045-25 .....137	148-0081-25 .....80	162-0036-18.....173	164-0070-18.....40
144-1530-20 .....137	144-2045-30 .....137	148-0081-25 .....161	162-0036-22.....173	164-0070-20.....24
144-1530-25 .....137	144-2050-15 .....137	148-0081-25 .....199	162-0040-30.....178	164-0070-20.....199
144-1530-30 .....137	144-2050-20 .....137	148-0081-27.....199	162-0040-35.....178	164-0070-24.....199
144-1535-15.....137	144-2050-25 .....137	148-0081-30.....199	162-0112-02.....167	164-0070-27.....24
144-1535-20 .....137	144-2050-30 .....137	148-0081-32.....199	162-0112-02.....169	164-0070-27.....40
144-1535-25 .....137	144-2060-15 .....137	148-0081-35.....199	162-0146-02.....167	164-0070-27.....199
144-1535-30 .....137	144-2060-20 .....137	148-0081-45.....199	162-0146-02.....169	164-0070-35.....24
144-1540-15 .....137	144-2060-25 .....137	148-0084-18.....149	162-0150-11.....172	164-0070-35.....40
144-1540-20 .....137	144-2060-30 .....137	148-0084-18.....199	162-0169-30.....167	164-0070-35.....199
144-1540-25 .....137	144-8888-20.....152	148-0084-23.....149	162-0169-30.....169	164-0071-15.....79
144-1540-30 .....137	144-8888-24.....152	148-0084-23.....199	162-0182-27.....167	164-0071-15.....199
144-2008-10 .....137	144-8888-27.....152	148-0084-27.....149	162-0182-27.....169	164-1013-20.....115
144-2008-15 .....137	144-8888-35.....152	148-0084-27.....199	162-0195-34.....172	164-1013-20.....201
144-2008-20 .....137	148-0080-07.....114	148-0084-38.....149	162-0197-27.....167	164-1520-20.....24
144-2010-10 .....137	148-0080-07.....199	148-0084-38.....199	162-0197-27.....169	164-1520-20.....32
144-2010-15 .....137	148-0080-10.....114	148-0180-11.....114	162-1124-30.....173	164-1520-20.....79
144-2010-20 .....137	148-0080-10.....199	148-0180-11.....199	162-1131-65.....173	164-1520-20.....115
144-2010-25 .....137	148-0080-11.....25	148-0180-15.....114	162-1135-22.....173	164-1520-20.... 201
144-2010-30 .....137	148-0080-11.....114	148-0180-15.....199	162-1136-22.....173	164-1600-00.... 148
144-2012-10.....137	148-0080-11.....199	148-0181-11.....114	163-200-20.....176	164-1600-00.....201
144-2012-15.....137	148-0080-15.....25	148-0181-11.....199	163-404-755.....179	164-2000-00.....79
144-2012-20.....137	148-0080-15.....33	148-0181-15.....114	163-404-756.....179	164-2000-00.....115
144-2012-25.....137	148-0080-15.....80	148-0181-15.....199	163-404-768.....179	164-2000-00.... 200
144-2012-30 .....137	148-0080-15.....114	148-0650-20.....193	163-404-782.....179	164-2400-00.....79
144-2014-10.....137	148-0080-15.....199	148-0650-30.....193	163-404-784.....179	164-2400-00.....115
144-2014-15.....137	148-0080-18.....25	148-0650-50.....193	163-404-791.....179	164-2400-00.... 200
144-2014-20 .....137	148-0080-18.....33	148-0651-17.....193	163-404-792.....179	164-2700-00.....79
144-2014-25 .....137	148-0080-18.....40	148-0651-30.....193	163-404-794.....179	164-2700-00.....115
144-2014-30 .....137	148-0080-18.....80	148-1050-03.....141	163-404-795.....179	164-2700-00.... 200
144-2015-10.....137	148-0080-18.....114	148-1050-05.....141	163-404-802.....179	164-2735-60.....24
144-2015-15.....137	148-0080-18.....199	148-1050-08.....141	163-404-812.....179	164-2735-60.....32
144-2015-20 .....137	148-0080-20.....25	150-0300-10.....210	163-500-28.....178	164-2735-60.....40
144-2015-25 .....137	148-0080-20.....40	150-0515-00.....198	163-501-28.....178	164-2735-60.....79

164-2735-60 .....115	170-1086-06 .... 207	230-2162-316 .....37	242-124-06.....132	242-127-24 .....132
164-2735-60 .....201	170-1087-07 .... 207	230-2162-319 .....37	242-124-08.....49	242-127-26 .....51
164-3500-00.....79	170-1088-08 .... 207	230-2162-616 .....37	242-124-08..... 108	242-127-26 ..... 108
164-3500-00.....115	170-1090-10 .... 207	230-2162-619 .....37	242-124-08.....132	242-127-26 .....132
164-3500-00.... 200	170-1092-12..... 207	230-2162-622 .....37	242-124-10 .....49	242-127-28 .....51
165-0100-00.....167	170-1104-04 .... 207	230-2162-919 .....37	242-124-10 ..... 108	242-127-28 ..... 108
165-0100-00.....173	170-1105-06 .... 207	230-2162-922 .....37	242-124-10 .....132	242-127-28 .....132
165-0100-21 .....167	170-1114-04..... 207	230-2162-925 .....37	242-124-12 .....49	242-127-30 .....51
165-0100-21 .....174	170-1115-06..... 207	230-2162-1222 ....37	242-124-12 ..... 108	242-127-30 ..... 108
165-0100-27 .....167	170-1120-06 .... 207	230-2162-1225 ....37	242-124-12 .....132	242-127-30 .....132
165-0100-27 .....174	170-1124-04..... 207	230-2162-1228 ....37	242-124-14 .....49	242-127-32 .....51
165-0100-34 .....167	170-1125-06..... 207	230-2162-1525 ....37	242-124-14 ..... 108	242-127-32 ..... 108
165-0100-34 .....174	170-1135-05..... 208	230-2162-1528 ....37	242-124-14 .....132	242-127-32 .....132
165-0110-10.....171	170-1137-25..... 208	230-2162-1531 ....37	242-124-16 .....49	242-127-34 .....51
165-0110-15.....167	170-1140-01..... 208	230-2162-4512 ....37	242-124-16 ..... 108	242-127-34 ..... 108
165-0110-15.....171	170-1142-02..... 208	230-2162-4515 ....37	242-124-16 .....132	242-127-34 .....132
165-0110-23 .....167	170-1145-03..... 208	230-2162-4518 ....37	242-124-18 .....49	242-127-36 .....51
165-0110-23 .....171	170-1146-04 .... 208	230-2162-7513 ....37	242-124-18 ..... 108	242-127-36 ..... 108
165-0120-15 .....167	170-1150-05..... 208	230-2162-7516 ....37	242-124-18 .....132	242-127-36 .....132
165-0120-15 .....171	170-1155-02..... 208	230-2162-7519 ....37	242-124-20 .....49	242-127-38 .....51
165-0120-28 .....171	170-1156-03..... 208	230-2162-7522 ....37	242-124-20 ..... 108	242-127-38 ..... 108
165-0120-30 .....171	170-1157-04..... 208	230-2162-10519 ...37	242-124-20 .....132	242-127-38 .....132
165-0130-00 .....171	170-1158-05..... 208	230-2162-10522 ...37	242-124-22 .....49	242-127-40 .....51
165-0130-22 .....171	170-1170-01..... 206	230-2162-10525 ...37	242-124-22 ..... 108	242-127-40 ..... 108
165-0130-25 .....171	170-1210-03 .... 208	230-2163-622 .....37	242-124-22 .....132	242-127-40 .....132
165-0140-00 .....171	170-1211-02..... 208	230-2163-926 .....37	242-124-24 .....49	242-127-42 .....51
165-0150-32 .....167	170-1212-07..... 208	230-2163-1230 ....37	242-124-24 ..... 108	242-127-42 ..... 108
165-0150-32 .....174	170-1215-06..... 208	230-2163-1532 ....37	242-124-24 .....132	242-127-42 .....132
165-5003-00 .....174	170-1216-04 .... 208	230-2163-7524 ....37	242-124-26 .....49	242-127-44 .....51
169-1500-00 .....212	170-1218-05..... 208	230-2163-10528 ...37	242-124-26 ..... 108	242-127-44 ..... 108
169-1500-01 .....212	170-1220-08 .... 209	242-0020-24 .... 109	242-124-26 .....132	242-127-44 .....132
169-1500-03 .....213	170-1222-08 .... 209	242-0027-35 .... 109	242-124-28 .....49	242-127-46 .....51
169-1520-04 .....213	170-1223-08 .... 209	242-120-06.....49	242-124-28 ..... 108	242-127-46 ..... 108
169-1520-06 .....213	170-1225-07 .... 206	242-120-06..... 108	242-124-28 .....132	242-127-46 .....132
169-1537-03.....213	170-1232-04 .... 209	242-120-06.....132	242-124-30 .....49	242-127-48 .....51
169-1562-02 .....213	170-1233-04 .... 209	242-120-08.....49	242-124-30 ..... 108	242-127-48 ..... 108
169-1562-03 .....213	170-1234-04 .... 209	242-120-08..... 108	242-124-30 .....132	242-127-48 .....132
169-1562-04 .....213	170-1235-06 .... 206	242-120-08.....132	242-124-32 ..... 108	242-127-50 .....51
169-1562-05 .....213	170-1236-04 .... 206	242-120-10.....49	242-124-32 .....132	242-127-50 ..... 108
169-1562-06 .....213	170-1266-06 .... 209	242-120-10..... 108	242-124-34 ..... 108	242-127-50 .....132
169-1562-07 .....213	170-1268-08 .... 209	242-120-10.....132	242-124-34 .....132	242-135-10 .....51
169-1562-08 .....213	170-1269-08 .... 209	242-120-12 .....49	242-124-36 ..... 108	242-135-10 ..... 108
169-1562-09 .....213	170-1270-10..... 209	242-120-12 ..... 108	242-124-36 .....132	242-135-10 .....132
169-1562-10.....213	170-1273-12..... 209	242-120-12 .....132	242-124-38 ..... 108	242-135-12 .....51
169-1570-52 .....213	170-1300-03 .... 209	242-120-14 .....49	242-124-38 .....132	242-135-12 ..... 108
169-1580-20 .....213	170-1305-03 .... 209	242-120-14 ..... 108	242-124-40 ..... 108	242-135-12 .....132
170-1005-04 .... 209	230-155-03 .....37	242-120-14 .....132	242-124-40 .....132	242-135-14 .....51
170-1005-06 .... 209	230-155-04 .....37	242-120-16 .....49	242-127-10 .....51	242-135-14 ..... 108
170-1010-09 .... 209	230-155-05 .....37	242-120-16 ..... 108	242-127-10 ..... 108	242-135-14 .....132
170-1025-02 .... 206	230-155-06 .....37	242-120-16 .....132	242-127-10 .....132	242-135-16 .....51
170-1029-06 .... 206	230-155-07 .....37	242-120-18 .....49	242-127-12 .....51	242-135-16 ..... 108
170-1030-07 .... 206	230-155-08 .....37	242-120-18 ..... 108	242-127-12 ..... 108	242-135-16 .....132
170-1031-08 .... 206	230-2020-00 .....36	242-120-18 .....132	242-127-12 .....132	242-135-18 .....51
170-1037-03..... 206	230-2040-00 .....36	242-120-20 .....49	242-127-14 .....51	242-135-18 ..... 108
170-1038-03 .... 206	230-2080-00 .....36	242-120-20 ..... 108	242-127-14 ..... 108	242-135-18 .....132
170-1040-02 ..... 207	230-2080-00 .....36	242-120-20 .....132	242-127-14 .....132	242-135-20 .....51
170-1045-03 .... 207	230-2160-03 .....37	242-120-22 .....49	242-127-16 .....51	242-135-20 ..... 108
170-1050-04 .... 207	230-2160-04 .....37	242-120-22 ..... 108	242-127-16 ..... 108	242-135-20 .....132
170-1055-05 .... 207	230-2160-05 .....37	242-120-22 .....132	242-127-16 .....132	242-135-22 .....51
170-1062-02 .....210	230-2160-06 .....37	242-120-24 .....49	242-127-18 .....51	242-135-22 ..... 108
170-1063-03 .....210	230-2160-07 .....37	242-120-24 ..... 108	242-127-18 ..... 108	242-135-22 .....132
170-1065-05 .....210	230-2160-08 .....37	242-120-24 .....132	242-127-18 .....132	242-135-24 .....51
170-1066-06 .....210	230-2161-03 .....37	242-120-26 ..... 108	242-127-20 .....51	242-135-24 ..... 108
170-1067-07 .....210	230-2161-04 .....37	242-120-26 .....132	242-127-20 ..... 108	242-135-24 .....132
170-1070-10.....210	230-2161-05 .....37	242-120-28 ..... 108	242-127-20 .....132	242-135-26 .....51
170-1072-12.....210	230-2161-06 .....37	242-120-28 .....132	242-127-22 .....51	242-135-26 ..... 108
170-1082-02 .... 207	230-2161-07 .....37	242-120-30 ..... 108	242-127-22 ..... 108	242-135-26 .....132
170-1083-03 .... 207	230-2161-08 .....37	242-120-30 .....132	242-127-22 .....132	242-135-28 .....51
170-1084-04 .... 207	230-2162-310 .....37	242-124-06.....49	242-127-24 .....51	242-135-28 ..... 108
170-1085-05 .... 207	230-2162-313 .....37	242-124-06..... 108	242-127-24 ..... 108	242-135-28 .....132

242-135-30.....51	242-220-08 .....131	242-224-18.....65	242-227-20.....131	242-235-14.....67
242-135-30.....108	242-220-10.....55	242-224-18.....73	242-227-22.....57	242-235-14.....75
242-135-30.....132	242-220-10.....65	242-224-18.....131	242-227-22.....67	242-235-14.....131
242-135-32.....51	242-220-10.....73	242-224-20.....55	242-227-22.....75	242-235-16.....57
242-135-32.....108	242-220-10.....131	242-224-20.....65	242-227-22.....131	242-235-16.....67
242-135-32.....132	242-220-12.....55	242-224-20.....73	242-227-24.....57	242-235-16.....75
242-135-34.....51	242-220-12.....65	242-224-20.....131	242-227-24.....67	242-235-16.....131
242-135-34.....108	242-220-12.....73	242-224-22.....55	242-227-24.....75	242-235-18.....57
242-135-34.....132	242-220-12.....131	242-224-22.....65	242-227-24.....131	242-235-18.....67
242-135-36.....51	242-220-14.....55	242-224-22.....73	242-227-26.....57	242-235-18.....75
242-135-36.....108	242-220-14.....65	242-224-22.....131	242-227-26.....67	242-235-18.....131
242-135-36.....132	242-220-14.....73	242-224-24.....55	242-227-26.....75	242-235-20.....57
242-135-38.....51	242-220-14.....131	242-224-24.....65	242-227-26.....131	242-235-20.....67
242-135-38.....108	242-220-16.....55	242-224-24.....73	242-227-28.....57	242-235-20.....75
242-135-38.....132	242-220-16.....65	242-224-24.....131	242-227-28.....67	242-235-20.....131
242-135-40.....51	242-220-16.....73	242-224-26.....55	242-227-28.....75	242-235-22.....57
242-135-40.....108	242-220-16.....131	242-224-26.....65	242-227-28.....131	242-235-22.....67
242-135-40.....132	242-220-18.....55	242-224-26.....73	242-227-30.....57	242-235-22.....75
242-135-42.....51	242-220-18.....65	242-224-26.....131	242-227-30.....67	242-235-22.....131
242-135-42.....108	242-220-18.....73	242-224-28.....55	242-227-30.....75	242-235-24.....57
242-135-42.....132	242-220-18.....131	242-224-28.....65	242-227-30.....131	242-235-24.....67
242-135-44.....51	242-220-20.....55	242-224-28.....73	242-227-32.....57	242-235-24.....75
242-135-44.....108	242-220-20.....65	242-224-28.....131	242-227-32.....67	242-235-24.....131
242-135-44.....132	242-220-20.....73	242-224-30.....55	242-227-32.....75	242-235-26.....57
242-135-46.....51	242-220-20.....131	242-224-30.....65	242-227-32.....131	242-235-26.....67
242-135-46.....108	242-220-22.....55	242-224-30.....73	242-227-34.....57	242-235-26.....75
242-135-46.....132	242-220-22.....65	242-224-30.....131	242-227-34.....67	242-235-26.....131
242-135-48.....51	242-220-22.....73	242-224-32.....55	242-227-34.....75	242-235-28.....57
242-135-48.....108	242-220-22.....131	242-224-32.....65	242-227-34.....131	242-235-28.....67
242-135-48.....132	242-220-24.....55	242-224-32.....73	242-227-36.....57	242-235-28.....75
242-135-50.....51	242-220-24.....65	242-224-32.....131	242-227-36.....67	242-235-28.....131
242-135-50.....108	242-220-24.....73	242-224-34.....55	242-227-36.....75	242-235-30.....57
242-135-50.....132	242-220-24.....131	242-224-34.....65	242-227-36.....131	242-235-30.....67
242-135-52.....51	242-220-26.....55	242-224-34.....73	242-227-38.....57	242-235-30.....75
242-135-52.....108	242-220-26.....65	242-224-34.....131	242-227-38.....67	242-235-30.....131
242-135-52.....132	242-220-26.....73	242-224-36.....55	242-227-38.....75	242-235-32.....57
242-135-54.....51	242-220-26.....131	242-224-36.....65	242-227-38.....131	242-235-32.....67
242-135-54.....108	242-220-28.....55	242-224-36.....73	242-227-40.....57	242-235-32.....75
242-135-54.....132	242-220-28.....65	242-224-36.....131	242-227-40.....67	242-235-32.....131
242-135-56.....51	242-220-28.....73	242-224-38.....55	242-227-40.....75	242-235-34.....57
242-135-56.....108	242-220-28.....131	242-224-38.....65	242-227-40.....131	242-235-34.....67
242-135-56.....132	242-220-30.....55	242-224-38.....73	242-227-42.....57	242-235-34.....75
242-135-58.....51	242-220-30.....65	242-224-38.....131	242-227-42.....67	242-235-34.....131
242-135-58.....108	242-220-30.....73	242-224-40.....55	242-227-42.....75	242-235-36.....57
242-135-58.....132	242-220-30.....131	242-224-40.....65	242-227-42.....131	242-235-36.....67
242-135-60.....51	242-224-06.....55	242-224-40.....73	242-227-44.....57	242-235-36.....75
242-135-60.....108	242-224-06.....65	242-224-40.....131	242-227-44.....67	242-235-36.....131
242-135-60.....132	242-224-06.....73	242-227-10.....57	242-227-44.....75	242-235-38.....57
242-135-62.....51	242-224-06.....131	242-227-10.....67	242-227-44.....131	242-235-38.....67
242-135-62.....108	242-224-08.....55	242-227-10.....75	242-227-46.....57	242-235-38.....75
242-135-62.....132	242-224-08.....65	242-227-10.....131	242-227-46.....67	242-235-38.....131
242-135-64.....51	242-224-08.....73	242-227-12.....57	242-227-46.....75	242-235-40.....57
242-135-64.....108	242-224-08.....131	242-227-12.....67	242-227-46.....131	242-235-40.....67
242-135-64.....132	242-224-10.....55	242-227-12.....75	242-227-48.....57	242-235-40.....75
242-135-66.....51	242-224-10.....65	242-227-12.....131	242-227-48.....67	242-235-40.....131
242-135-66.....108	242-224-10.....73	242-227-14.....57	242-227-48.....75	242-235-42.....57
242-135-66.....132	242-224-10.....131	242-227-14.....67	242-227-48.....131	242-235-42.....67
242-135-68.....51	242-224-12.....55	242-227-14.....75	242-227-50.....57	242-235-42.....75
242-135-68.....108	242-224-12.....65	242-227-14.....131	242-227-50.....67	242-235-42.....131
242-135-68.....132	242-224-12.....73	242-227-16.....57	242-227-50.....75	242-235-44.....57
242-135-70.....51	242-224-12.....131	242-227-16.....67	242-227-50.....131	242-235-44.....67
242-135-70.....108	242-224-14.....55	242-227-16.....75	242-235-10.....57	242-235-44.....75
242-135-70.....132	242-224-14.....65	242-227-16.....131	242-235-10.....67	242-235-44.....131
242-220-06.....55	242-224-14.....73	242-227-18.....57	242-235-10.....75	242-235-46.....57
242-220-06.....65	242-224-14.....131	242-227-18.....67	242-235-10.....131	242-235-46.....67
242-220-06.....73	242-224-16.....55	242-227-18.....75	242-235-12.....57	242-235-46.....75
242-220-06.....131	242-224-16.....65	242-227-18.....131	242-235-12.....67	242-235-46.....131
242-220-08.....55	242-224-16.....73	242-227-20.....57	242-235-12.....75	242-235-48.....57
242-220-08.....65	242-224-16.....131	242-227-20.....67	242-235-12.....131	242-235-48.....67
242-220-08.....73	242-224-18.....55	242-227-20.....75	242-235-14.....57	242-235-48.....75

242-235-48 .....131	244-4050-45.....147	245-127-08.....127	245-140-60 .....129	245-220-22 .....20
242-235-50.....57	244-4050-50.....147	245-127-10.....127	245-140-62 .....129	245-220-22 .....31
242-235-50.....67	244-4050-55.....147	245-127-12.....127	245-140-64 .....129	245-220-22 .....126
242-235-50.....75	244-4050-60.....147	245-127-14.....127	245-140-66 .....129	245-220-24 .....20
242-235-50.....131	244-4060-10.....147	245-127-16.....127	245-140-68 .....129	245-220-24 .....31
242-235-52.....57	244-5060-20.....147	245-127-18.....127	245-140-70.....129	245-220-24 .....126
242-235-52.....67	244-5060-22.....147	245-127-20.....127	245-145-14.....129	245-220-26 .....20
242-235-52.....75	244-5060-24.....147	245-127-22.....127	245-145-16.....129	245-220-26 .....31
242-235-52.....131	244-5060-26.....147	245-127-24.....127	245-145-18.....129	245-220-26 .....126
242-235-54.....57	244-5060-28.....147	245-127-26.....127	245-145-20.....129	245-220-28 .....20
242-235-54.....67	244-5060-30.....147	245-127-28.....127	245-145-22.....129	245-220-28 .....31
242-235-54.....75	244-5060-32.....147	245-127-30.....127	245-145-24.....129	245-220-28 .....126
242-235-54.....131	244-5060-34.....147	245-127-32.....127	245-145-26.....129	245-220-30 .....20
242-235-56.....57	244-5060-36.....147	245-127-34.....127	245-145-28.....129	245-220-30 .....31
242-235-56.....67	244-5060-38.....147	245-127-36.....127	245-145-30.....129	245-220-30 .....126
242-235-56.....75	244-5060-40.....147	245-127-38.....127	245-145-32.....129	245-224-06 .....20
242-235-56.....131	244-5060-45.....147	245-127-40.....127	245-145-34.....129	245-224-06 .....31
242-235-58.....57	244-5060-50.....147	245-127-42.....127	245-145-36.....129	245-224-06 .....38
242-235-58.....67	244-5060-55.....147	245-135-08 .....128	245-145-38.....129	245-224-06 .....127
242-235-58.....75	244-5060-60.....147	245-135-10.....128	245-145-40 .....129	245-224-08 .....20
242-235-58.....131	245-115-06.....126	245-135-12.....128	245-145-42.....129	245-224-08 .....31
242-235-60 .....57	245-115-07.....126	245-135-14.....128	245-145-44 .....129	245-224-08 .....38
242-235-60 .....67	245-115-08.....126	245-135-16.....128	245-145-46 .....129	245-224-08 .....127
242-235-60 .....75	245-115-09.....126	245-135-18.....128	245-145-48 .....129	245-224-10.....20
242-235-60 .....131	245-115-10.....126	245-135-20.....128	245-145-50.....129	245-224-10.....31
244-2431-08 .... 146	245-115-11.....126	245-135-22.....128	245-145-52.....129	245-224-10.....38
244-2431-10..... 146	245-115-12.....126	245-135-24.....128	245-145-54.....129	245-224-10.....127
244-2431-12..... 146	245-115-14.....126	245-135-26.....128	245-145-56.....129	245-224-12.....20
244-2431-14..... 146	245-115-16.....126	245-135-28.....128	245-145-58.....129	245-224-12.....31
244-2431-16..... 146	245-115-18.....126	245-135-30.....128	245-145-60.....129	245-224-12.....38
244-2431-18..... 146	245-115-20.....126	245-135-32.....128	245-145-62 .....129	245-224-12.....127
244-2431-20 .... 146	245-120-06 .....126	245-135-34.....128	245-145-64 .....129	245-224-14.....20
244-2431-22 .... 146	245-120-08 .....126	245-135-36.....128	245-145-66 .....129	245-224-14.....31
244-2431-24..... 146	245-120-10.....126	245-135-38.....128	245-145-68 .....129	245-224-14.....38
244-2431-26 .... 146	245-120-12.....126	245-135-40 .....128	245-145-70.....129	245-224-14.....127
244-2431-28 .... 146	245-120-14.....126	245-135-42.....128	245-215-06 .....126	245-224-16.....20
244-2431-30 .... 146	245-120-16.....126	245-135-44 .....128	245-215-07.....126	245-224-16.....31
244-2439-00 .... 146	245-120-18.....126	245-135-45.....128	245-215-08 .....126	245-224-16.....38
244-2439-10 .... 146	245-120-20.....126	245-135-50.....128	245-215-09.....126	245-224-16.....127
244-2460-10 .....145	245-120-22.....126	245-135-55.....128	245-215-10.....126	245-224-18.....20
244-3039-10 .... 146	245-120-24.....126	245-135-60 .....128	245-215-11 .....126	245-224-18.....31
244-3039-12 .... 146	245-120-26.....126	245-135-65.....128	245-215-12 .....126	245-224-18.....38
244-3039-14 .... 146	245-120-28.....126	245-140-10.....129	245-215-14 .....126	245-224-18.....127
244-3039-16 .... 146	245-120-30.....126	245-140-12.....129	245-215-16 .....126	245-224-20.....20
244-3039-18 .... 146	245-120-32.....126	245-140-14.....129	245-215-18 .....126	245-224-20.....31
244-3039-20 .... 146	245-120-34.....126	245-140-16.....129	245-215-20.....126	245-224-20.....38
244-3039-22 ..... 146	245-120-36.....126	245-140-18.....129	245-220-06 .....20	245-224-20.....127
244-3039-24 ..... 146	245-120-38.....126	245-140-20.....129	245-220-06 .....31	245-224-22 .....20
244-3039-26 .... 146	245-120-40 .....126	245-140-22.....129	245-220-06 .....126	245-224-22 .....31
244-3039-28 .... 146	245-120-42.....126	245-140-24.....129	245-220-08 .....20	245-224-22 .....38
244-3039-30 .... 146	245-120-44 .....126	245-140-26.....129	245-220-08 .....31	245-224-22 .....127
244-3039-32 .... 146	245-124-06 .....127	245-140-28.....129	245-220-08 .....126	245-224-24.....20
244-3039-34 .... 146	245-124-08 .....127	245-140-30 .....129	245-220-10.....20	245-224-24.....31
244-3039-36 .... 146	245-124-10.....127	245-140-32.....129	245-220-10.....31	245-224-24.....38
244-3039-38 .... 146	245-124-12.....127	245-140-34 .....129	245-220-10.....126	245-224-24.....127
244-3039-40 ..... 146	245-124-14.....127	245-140-35.....129	245-220-12.....20	245-224-26.....20
244-4050-14 .....147	245-124-16.....127	245-140-36 .....129	245-220-12.....31	245-224-26.....31
244-4050-16 .....147	245-124-18.....127	245-140-38 .....129	245-220-12.....126	245-224-26.....38
244-4050-18 .....147	245-124-20.....127	245-140-40 .....129	245-220-14.....20	245-224-26.....127
244-4050-20 .....147	245-124-22.....127	245-140-42 .....129	245-220-14.....31	245-224-28.....20
244-4050-22 .....147	245-124-24.....127	245-140-44 .....129	245-220-14.....126	245-224-28.....31
244-4050-24 .....147	245-124-26.....127	245-140-45 .....129	245-220-16.....20	245-224-28.....38
244-4050-26 .....147	245-124-28.....127	245-140-46 .....129	245-220-16.....31	245-224-28.....127
244-4050-28 .....147	245-124-30.....127	245-140-48 .....129	245-220-16.....126	245-224-30 .....20
244-4050-30.....147	245-124-32.....127	245-140-50 .....129	245-220-18.....20	245-224-30 .....31
244-4050-32.....147	245-124-34.....127	245-140-52 .....129	245-220-18.....31	245-224-30 .....38
244-4050-34 .....147	245-124-36.....127	245-140-54 .....129	245-220-18.....126	245-224-30 .....127
244-4050-36 .....147	245-124-38.....127	245-140-55.....129	245-220-20 .....20	245-224-32 .....20
244-4050-38 .....147	245-124-40 .....127	245-140-56 .....129	245-220-20 .....31	245-224-32 .....31
244-4050-40.....147	245-127-06.....127	245-140-58 .....129	245-220-20 .....126	245-224-32 .....38

245-224-32 .....127	245-235-24.....128	245-413-18.....130	245-427-10..... 160	245-520-07 .....31
245-224-34 .....20	245-235-26.....39	245-413-20.....85	245-427-12.....130	245-520-07 .....126
245-224-34 .....31	245-235-26.....128	245-413-20.....130	245-427-12..... 160	245-520-08 .....20
245-224-34 .....38	245-235-28.....39	245-415-05 .....91	245-427-14.....130	245-520-08 .....31
245-224-34 .....127	245-235-28.....128	245-415-05 .....130	245-427-14..... 160	245-520-08 .....55
245-224-36 .....20	245-235-30 .....39	245-415-06 .....91	245-427-16.....130	245-520-08 .....65
245-224-36 .....31	245-235-30 .....128	245-415-06 .....130	245-427-16..... 160	245-520-08 .....73
245-224-36 .....38	245-235-32.....39	245-415-07 .....91	245-427-18.....130	245-520-08 .....126
245-224-36 .....127	245-235-32.....128	245-415-07 .....130	245-427-18..... 160	245-520-09 .....31
245-224-38 .....20	245-235-34 .....39	245-415-08 .....91	245-427-20.....130	245-520-09 .....126
245-224-38 .....31	245-235-34 .....128	245-415-08 .....130	245-427-20..... 160	245-520-10.....20
245-224-38 .....38	245-235-36 .....39	245-415-09 .....91	245-440-10 .....129	245-520-10.....31
245-224-38 .....127	245-235-36 .....128	245-415-09 .....130	245-440-12 .....129	245-520-10.....55
245-224-40 .....20	245-235-38 .....39	245-415-10 .....91	245-440-14 .....129	245-520-10.....65
245-224-40 .....31	245-235-38 .....128	245-415-10 .....130	245-440-16 .....129	245-520-10.....73
245-224-40 .....38	245-235-40 .....39	245-415-11 .....91	245-440-18 .....129	245-520-10.....126
245-224-40 .....127	245-235-40 .....128	245-415-11 .....130	245-440-20 .....129	245-520-12.....20
245-227-06 .....39	245-235-45 .....39	245-415-12 .....91	245-440-22 .....129	245-520-12.....31
245-227-06 .....127	245-235-45 .....128	245-415-12 .....130	245-440-24 .....129	245-520-12.....55
245-227-08 .....39	245-235-50 .....39	245-415-14 .....91	245-440-26 .....129	245-520-12.....65
245-227-08 .....127	245-235-50 .....128	245-415-14 .....130	245-440-28 .....129	245-520-12.....73
245-227-10 .....39	245-235-55 .....39	245-415-16 .....91	245-440-30 .....129	245-520-12.....126
245-227-10 .....127	245-235-55 .....128	245-415-16 .....130	245-440-32 .....129	245-520-14.....20
245-227-12.....39	245-235-60 .....39	245-415-18 .....91	245-440-34 .....129	245-520-14.....31
245-227-12.....127	245-235-60 .....128	245-415-18 .....130	245-440-35 .....129	245-520-14.....55
245-227-14.....39	245-410-04 .....85	245-415-20 .....91	245-440-36 .....129	245-520-14.....65
245-227-14.....127	245-410-04 .....130	245-415-20 .....130	245-440-38 .....129	245-520-14.....73
245-227-16.....39	245-410-05 .....85	245-415-22 .....91	245-440-40 .....129	245-520-14.....126
245-227-16.....127	245-410-05 .....130	245-415-22 .....130	245-440-42 .....129	245-520-16.....20
245-227-18.....39	245-410-06 .....85	245-415-24 .....91	245-440-44 .....129	245-520-16.....31
245-227-18.....127	245-410-06 .....130	245-415-24 .....130	245-440-46 .....129	245-520-16.....55
245-227-20.....39	245-410-07 .....85	245-415-26 .....91	245-440-48 .....129	245-520-16.....65
245-227-20.....127	245-410-07 .....130	245-415-26 .....130	245-440-50 .....129	245-520-16.....73
245-227-22.....39	245-410-08 .....85	245-420-05 .....93	245-440-52 .....129	245-520-16.....126
245-227-22.....127	245-410-08 .....130	245-420-05 .....130	245-440-54 .....129	245-520-18.....20
245-227-24.....39	245-410-09 .....85	245-420-06 .....93	245-440-55 .....129	245-520-18.....31
245-227-24.....127	245-410-09 .....130	245-420-06 .....130	245-440-56 .....129	245-520-18.....55
245-227-26.....39	245-410-10 .....85	245-420-07 .....93	245-440-58 .....129	245-520-18.....65
245-227-26.....127	245-410-10 .....130	245-420-07 .....130	245-440-60 .....129	245-520-18.....73
245-227-28.....39	245-410-11 .....85	245-420-08 .....93	245-440-62 .....129	245-520-18.....126
245-227-28.....127	245-410-11 .....130	245-420-08 .....130	245-440-64 .....129	245-520-20 .....20
245-227-30.....39	245-410-12 .....85	245-420-09 .....93	245-440-66 .....129	245-520-20 .....31
245-227-30.....127	245-410-12 .....130	245-420-09 .....130	245-440-68 .....129	245-520-20 .....126
245-227-32.....39	245-410-14 .....85	245-420-10 .....93	245-440-70 .....129	245-520-22 .....20
245-227-32.....127	245-410-14 .....130	245-420-10 .....130	245-515-05 .....126	245-520-22 .....31
245-227-34.....39	245-410-16 .....85	245-420-11 .....93	245-515-06 .....20	245-520-22 .....126
245-227-34.....127	245-410-16 .....130	245-420-11 .....130	245-515-06 .....126	245-520-24 .....20
245-227-36.....39	245-413-04 .....85	245-420-12 .....93	245-515-07 .....20	245-520-24 .....31
245-227-36.....127	245-413-04 .....130	245-420-12 .....130	245-515-07 .....126	245-520-24 .....126
245-227-38.....39	245-413-05 .....85	245-420-14 .....93	245-515-08 .....20	245-520-26 .....20
245-227-38.....127	245-413-05 .....130	245-420-14 .....130	245-515-08 .....126	245-520-26 .....31
245-227-40 .....39	245-413-06 .....85	245-420-16 .....93	245-515-09 .....20	245-520-26 .....126
245-227-40 .....127	245-413-06 .....130	245-420-16 .....130	245-515-09 .....126	245-520-28 .....20
245-235-08 .....39	245-413-07 .....85	245-420-18 .....93	245-515-10 .....20	245-520-28 .....31
245-235-08 .....128	245-413-07 .....130	245-420-18 .....130	245-515-10 .....126	245-520-28 .....126
245-235-10.....39	245-413-08 .....85	245-420-20 .....93	245-515-12 .....20	245-520-30 .....20
245-235-10.....128	245-413-08 .....130	245-420-20 .....130	245-515-12 .....126	245-520-30 .....31
245-235-12.....39	245-413-09 .....85	245-420-22 .....93	245-515-14 .....20	245-520-30 .....126
245-235-12.....128	245-413-09 .....130	245-420-22 .....130	245-515-14 .....126	245-524-06 .....20
245-235-14.....39	245-413-10 .....85	245-420-24 .....93	245-515-16 .....20	245-524-06 .....31
245-235-14.....128	245-413-10 .....130	245-420-24 .....130	245-515-16 .....126	245-524-06 .....38
245-235-16.....39	245-413-11 .....85	245-420-26 .....93	245-515-18 .....20	245-524-06 .....127
245-235-16.....128	245-413-11 .....130	245-420-26 .....130	245-515-18 .....126	245-524-08 .....20
245-235-18.....39	245-413-12 .....85	245-420-28 .....93	245-515-20 .....20	245-524-08 .....31
245-235-18.....128	245-413-12 .....130	245-420-28 .....130	245-515-20 .....126	245-524-08 .....38
245-235-20.....39	245-413-14 .....85	245-420-30 .....93	245-520-05 .....31	245-524-08 .....55
245-235-20.....128	245-413-14 .....130	245-420-30 .....130	245-520-05 .....126	245-524-08 .....65
245-235-22.....39	245-413-16 .....85	245-427-08 .....130	245-520-06 .....20	245-524-08 .....73
245-235-22.....128	245-413-16 .....130	245-427-08 .....160	245-520-06 .....31	245-524-08 .....127
245-235-24.....39	245-413-18 .....85	245-427-10 .....130	245-520-06 .....126	245-524-10 .....20

245-524-10.....31	245-524-34 .....38	245-527-30.....39	245-535-28.....128	245-624-14 .....49
245-524-10.....38	245-524-34 .....127	245-527-30.....57	245-535-30 .....39	245-624-14 .....110
245-524-10.....55	245-524-36 .....20	245-527-30.....67	245-535-30 .....57	245-624-14 .....127
245-524-10.....65	245-524-36 .....31	245-527-30.....75	245-535-30 .....67	245-624-16 .....49
245-524-10.....73	245-524-36 .....38	245-527-30.....127	245-535-30 .....75	245-624-16 .....110
245-524-10.....127	245-524-36 .....127	245-527-32.....20	245-535-30 .....128	245-624-16 .....127
245-524-12.....20	245-524-38 .....20	245-527-32.....39	245-535-32 .....39	245-624-18 .....49
245-524-12.....31	245-524-38 .....31	245-527-32.....57	245-535-32 .....57	245-624-18 .....110
245-524-12.....38	245-524-38 .....38	245-527-32.....67	245-535-32 .....67	245-624-18 .....127
245-524-12.....55	245-524-38 .....127	245-527-32.....75	245-535-32 .....75	245-624-20 .....49
245-524-12.....65	245-524-40 .....20	245-527-32.....127	245-535-32 .....128	245-624-20 .....110
245-524-12.....73	245-524-40 .....31	245-527-34.....20	245-535-34 .....39	245-624-20 .....127
245-524-12.....127	245-524-40 .....38	245-527-34.....39	245-535-34 .....57	245-624-22 .....49
245-524-14.....20	245-524-40 .....127	245-527-34.....57	245-535-34 .....67	245-624-22 .....110
245-524-14.....31	245-527-06 .....39	245-527-34.....67	245-535-34 .....75	245-624-22 .....127
245-524-14.....38	245-527-06 .....127	245-527-34.....75	245-535-34 .....128	245-624-24 .....110
245-524-14.....55	245-527-08 .....39	245-527-34.....127	245-535-36 .....39	245-624-24 .....127
245-524-14.....65	245-527-08 .....127	245-527-36.....20	245-535-36 .....128	245-624-26 .....110
245-524-14.....73	245-527-10.....20	245-527-36.....39	245-535-38 .....39	245-624-26 .....127
245-524-14.....127	245-527-10.....39	245-527-36.....127	245-535-38 .....128	245-624-28 .....110
245-524-16.....20	245-527-10.....127	245-527-38.....20	245-535-40 .....39	245-624-28 .....127
245-524-16.....31	245-527-12.....20	245-527-38.....39	245-535-40 .....128	245-624-30 .....110
245-524-16.....38	245-527-12.....39	245-527-38.....127	245-535-45 .....39	245-624-30 .....127
245-524-16.....55	245-527-12.....127	245-527-40 .....20	245-535-45 .....128	245-624-32 .....110
245-524-16.....65	245-527-14.....20	245-527-40 .....39	245-535-50 .....39	245-624-32 .....127
245-524-16.....73	245-527-14.....39	245-527-40 .....127	245-535-50 .....128	245-624-34 .....110
245-524-16.....127	245-527-14.....127	245-527-45 .....20	245-535-55 .....39	245-624-34 .....127
245-524-18.....20	245-527-16.....20	245-527-45 .....127	245-535-55 .....128	245-624-36 .....110
245-524-18.....31	245-527-16.....39	245-527-50.....20	245-535-60 .....39	245-624-36 .....127
245-524-18.....38	245-527-16.....127	245-527-50.....127	245-535-60 .....128	245-624-38 .....110
245-524-18.....55	245-527-16.....67	245-535-08 .....128	245-620-06 .....126	245-624-38 .....127
245-524-18.....65	245-527-16.....75	245-535-10.....128	245-620-08 .....49	245-624-40 .....110
245-524-18.....73	245-527-16.....127	245-535-12.....39	245-620-08 .....110	245-624-40 .....127
245-524-18.....127	245-527-18.....20	245-535-12.....128	245-620-08 .....126	245-627-10.....127
245-524-20 .....20	245-527-18.....39	245-535-14.....39	245-620-10 .....49	245-627-12.....127
245-524-20 .....31	245-527-18.....57	245-535-14.....128	245-620-10 .....110	245-627-14.....127
245-524-20 .....38	245-527-18.....67	245-535-16.....39	245-620-10 .....126	245-627-16.....51
245-524-20 .....55	245-527-18.....75	245-535-16.....57	245-620-12 .....49	245-627-16.....110
245-524-20 .....65	245-527-18.....127	245-535-16.....67	245-620-12 .....110	245-627-16.....127
245-524-20 .....73	245-527-20.....20	245-535-16.....75	245-620-12 .....126	245-627-18.....51
245-524-20 .....127	245-527-20.....39	245-535-16.....128	245-620-14 .....49	245-627-18.....110
245-524-22 .....20	245-527-20.....57	245-535-18.....39	245-620-14 .....110	245-627-18.....127
245-524-22 .....31	245-527-20.....67	245-535-18.....57	245-620-14 .....126	245-627-20.....51
245-524-22 .....38	245-527-20.....75	245-535-18.....67	245-620-16 .....49	245-627-20.....110
245-524-22 .....55	245-527-20.....127	245-535-18.....75	245-620-16 .....110	245-627-20.....127
245-524-22 .....65	245-527-22.....20	245-535-18.....128	245-620-16 .....126	245-627-22 .....51
245-524-22 .....73	245-527-22.....39	245-535-20.....39	245-620-16 .....126	245-627-22 .....110
245-524-22 .....127	245-527-22.....57	245-535-20.....57	245-620-18 .....49	245-627-22 .....127
245-524-24.....20	245-527-22.....67	245-535-20.....67	245-620-18 .....110	245-627-24.....51
245-524-24.....31	245-527-22.....75	245-535-20.....75	245-620-18 .....126	245-627-24.....110
245-524-24.....38	245-527-22.....127	245-535-20.....128	245-620-20 .....126	245-627-24.....127
245-524-24.....127	245-527-24.....20	245-535-22 .....39	245-620-22 .....126	245-627-24.....127
245-524-26 .....20	245-527-24.....39	245-535-22 .....57	245-620-24 .....126	245-627-26.....51
245-524-26 .....31	245-527-24.....57	245-535-22 .....67	245-620-26 .....126	245-627-26.....110
245-524-26 .....38	245-527-24.....67	245-535-22 .....75	245-620-28 .....126	245-627-26.....127
245-524-26 .....127	245-527-24.....75	245-535-22 .....128	245-620-30 .....126	245-627-28 .....51
245-524-28 .....20	245-527-24.....127	245-535-24.....39	245-620-30 .....126	245-627-28 .....110
245-524-28 .....31	245-527-26.....20	245-535-24.....57	245-620-34 .....126	245-627-28 .....127
245-524-28 .....38	245-527-26.....39	245-535-24.....67	245-620-36 .....126	245-627-30 .....51
245-524-28 .....127	245-527-26.....57	245-535-24.....75	245-620-38 .....126	245-627-30 .....110
245-524-30 .....20	245-527-26.....67	245-535-24.....128	245-620-40 .....126	245-627-30 .....127
245-524-30 .....31	245-527-26.....75	245-535-26.....39	245-624-06 .....127	245-627-32 .....51
245-524-30 .....38	245-527-26.....127	245-535-26.....57	245-624-08 .....49	245-627-32 .....110
245-524-30 .....127	245-527-28.....20	245-535-26.....67	245-624-08 .....110	245-627-32 .....127
245-524-32 .....20	245-527-28.....39	245-535-26.....75	245-624-08 .....127	245-627-34 .....51
245-524-32 .....31	245-527-28.....57	245-535-26.....128	245-624-10 .....49	245-627-34 .....110
245-524-32 .....38	245-527-28.....67	245-535-28.....39	245-624-10 .....110	245-627-34 .....127
245-524-32 .....127	245-527-28.....75	245-535-28.....57	245-624-10 .....127	245-627-36 .....110
245-524-34 .....20	245-527-28.....127	245-535-28.....67	245-624-12 .....49	245-627-36 .....127
245-524-34 .....31	245-527-30.....20	245-535-28.....75	245-624-12 .....110	245-627-38 .....110
			245-624-12 .....127	245-627-38 .....127

245-627-40 .....	110	247-0102-00 ....	184
245-627-40 .....	127	247-0102-00 ....	196
245-635-08 .....	128	247-0102-00 ....	198
245-635-10 .....	128	247-0103-00 .....	25
245-635-12.....	128	247-0103-00 .....	33
245-635-14 .....	128	247-0103-00 .....	40
245-635-16 .....	51	247-0103-00 .....	80
245-635-16 .....	110	247-0103-00 .....	116
245-635-16 .....	128	247-0103-00 .....	198
245-635-18 .....	51	247-0104-00 .....	80
245-635-18 .....	110	247-0104-00 .....	116
245-635-18 .....	128	247-0104-00 ....	160
245-635-20 .....	51	247-0104-00 ....	198
245-635-20 .....	110	247-0105-00 ....	148
245-635-20 .....	128	247-0110-00 .....	196
245-635-22 .....	51	247-0112-00.....	196
245-635-22 .....	110	247-0113-00 .....	196
245-635-22 .....	128	247-0114-00 .....	196
245-635-24 .....	51	247-0115-00 .....	196
245-635-24 .....	110	247-0116-00 .....	196
245-635-24 .....	128	247-0117-00.....	196
245-635-26 .....	51	247-0120-00 .....	196
245-635-26 .....	110	247-0121-00 .....	196
245-635-26 .....	128	247-0122-00 .....	196
245-635-28 .....	51	247-0130-00 .....	196
245-635-28 .....	110	247-0131-00 .....	196
245-635-28 .....	128	247-0132-00 .....	196
245-635-30 .....	51	247-0133-00 .....	196
245-635-30 .....	110	247-0140-00 .....	196
245-635-30 .....	128	247-0141-00 .....	196
245-635-32 .....	51	247-0142-00 .....	196
245-635-32 .....	110	247-0143-00 .....	196
245-635-32 .....	128	247-0150-00 .....	196
245-635-34 .....	51	247-0151-00 .....	196
245-635-34 .....	110	247-0152-00 .....	196
245-635-34 .....	128	247-0160-00 .....	196
245-635-36 .....	110	247-0161-00 .....	196
245-635-36 .....	128	888-9500-10 .....	182
245-635-38 .....	110	888-9500-10 .....	182
245-635-38 .....	128	888-9501-00 .....	182
245-635-40 .....	110	888-9507-20 .....	182
245-635-40 .....	128	888-9507-20 .....	183
245-635-45 .....	110	888-9510-20 .....	182
245-635-45 .....	128	888-9510-20 .....	183
245-635-50 .....	110	888-9513-20 .....	182
245-635-50 .....	128	888-9513-20 .....	183
245-635-55 .....	110	888-9516-20 .....	182
245-635-55 .....	128	888-9516-20 .....	183
245-635-60 .....	110	888-9519-20 .....	182
245-635-60 .....	128	888-9519-20 .....	183
245-916-04 .....	141		
245-916-05 .....	141		
245-916-06 .....	141		
245-916-07 .....	141		
245-916-08 .....	141		
246-001-04 .....	40		
246-001-08 .....	40		
246-002-00 .....	40		
246-006-19 .....	40		
246-008-02.....	38		
246-008-04.....	38		
246-008-06.....	38		
247-0000-00.....	196		
247-0101-00 .....	182		
247-0101-00 ....	184		
247-0101-00 .....	196		
247-0102-00 .....	80		
247-0102-00 .....	116		
247-0102-00 ....	160		
247-0102-00 .....	182		

